

Specifications


| REF | Max. vessel diameter [mm] | Working length in max. vessel [mm]* | Min. vessel diameter [mm] | Working length in min. vessel [mm]* |
|------------|---------------------------|-------------------------------------|---------------------------|-------------------------------------|
| P64-250-9 | 2.5 | 9 | 2 | 13 |
| P64-300-9 | 3 | 9 | 2.5 | 12 |
| P64-300-12 | 3 | 12 | 2.5 | 16 |
| P64-300-15 | 3 | 15 | 2.5 | 21 |
| P64-350-9 | 3.5 | 9 | 3 | 13 |
| P64-350-12 | 3.5 | 12 | 3 | 17 |
| P64-350-15 | 3.5 | 15 | 3 | 21 |
| P64-350-18 | 3.5 | 18 | 3 | 25 |
| P64-350-21 | 3.5 | 21 | 3 | 29 |
| P64-400-12 | 4 | 12 | 3.5 | 13 |
| P64-400-15 | 4 | 15 | 3.5 | 17 |
| P64-400-18 | 4 | 18 | 3.5 | 21 |
| P64-400-21 | 4 | 21 | 3.5 | 25 |
| P64-400-24 | 4 | 24 | 3.5 | 28 |
| P64-400-27 | 4 | 27 | 3.5 | 32 |
| P64-450-15 | 4.5 | 15 | 4 | 22 |
| P64-450-18 | 4.5 | 18 | 4 | 25 |
| P64-450-21 | 4.5 | 21 | 4 | 29 |
| P64-450-24 | 4.5 | 24 | 4 | 33 |
| P64-450-27 | 4.5 | 27 | 4 | 40 |
| P64-500-18 | 5 | 18 | 4.5 | 20 |
| P64-500-24 | 5 | 24 | 4.5 | 28 |
| P64-500-30 | 5 | 30 | 4.5 | 37 |

*Working length is defined as: length of implant without proximal bundled implant ends, measured in silicone vessel without aneurysm neck.



p64
Flow Modulation Device

phenox

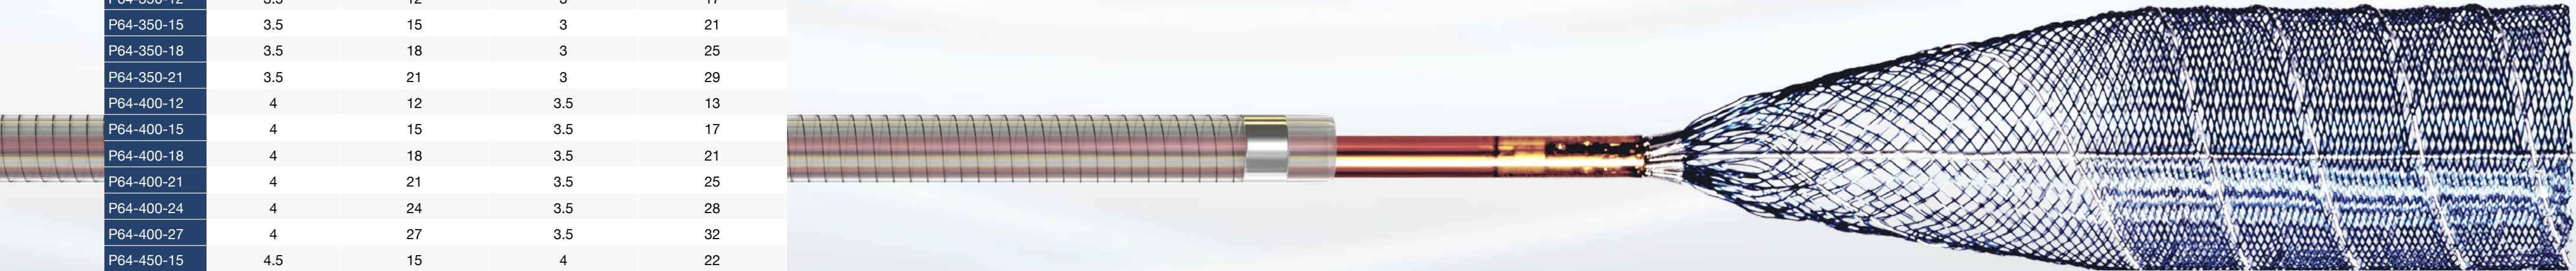


See the **p64** in action

Scan the QR-code or visit: <https://goo.gl/2dxQZc>



The power of safety and security -
Complete deployment with full recoverability



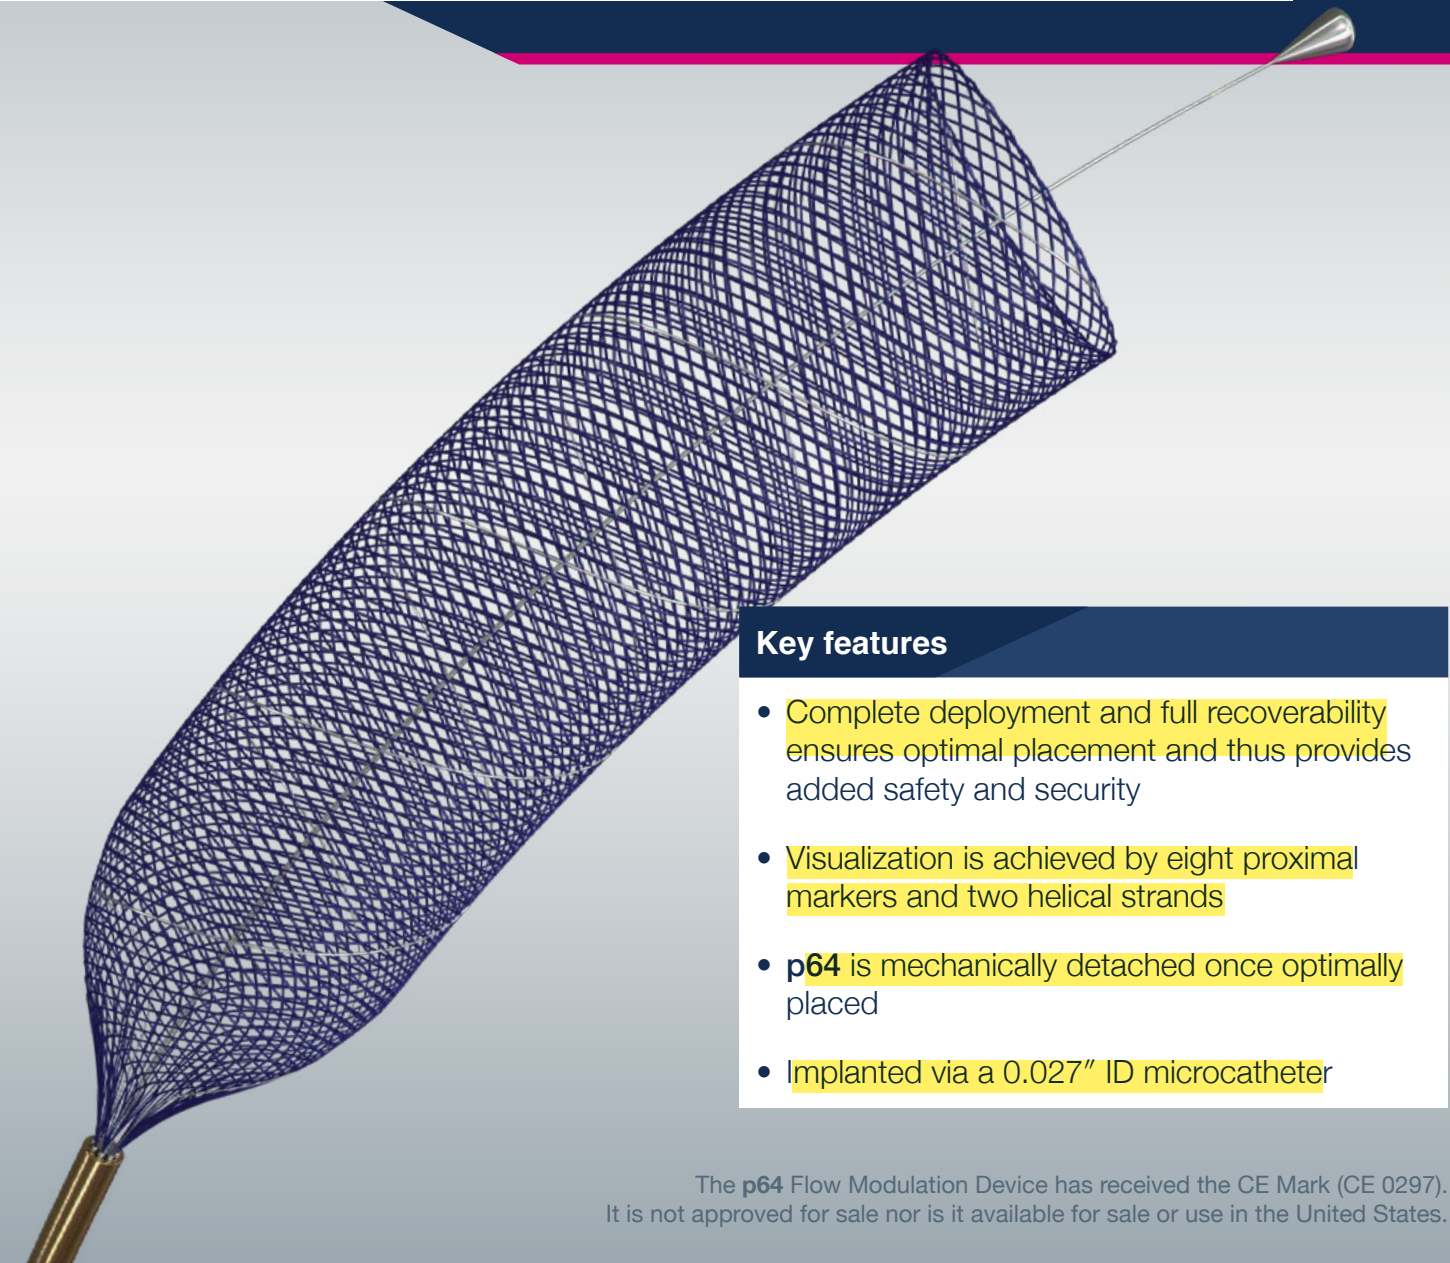


Key features

- Complete deployment and full recoverability ensures optimal placement and thus provides added safety and security
- Visualization is achieved by eight proximal markers and two helical strands
- p64 is mechanically detached once optimally placed
- Implanted via a 0.027" ID microcatheter

The **p64** Flow Modulation Device has received the CE Mark (CE 0297).
It is not approved for sale nor is it available for sale or use in the United States.

Ease of Use

p64 offers a new level of operator security and patient safety by allowing complete deployment with full recoverability.

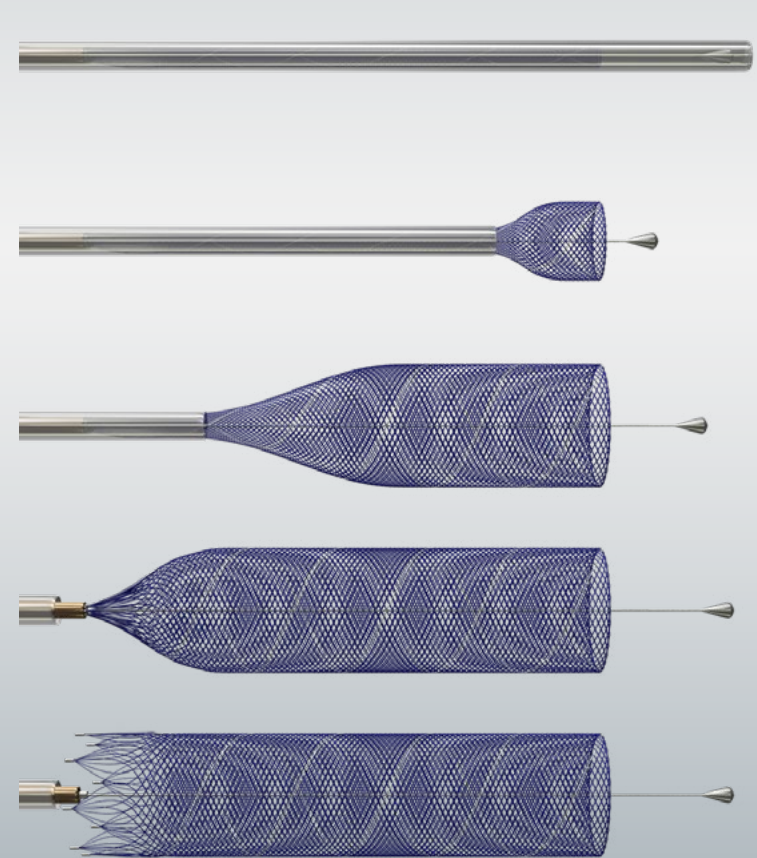

Neck Coverage

64 Nitinol wire braid leads to a dense aneurysm coverage and maximizes the hemodynamic flow effect in the vessel

150x magnification

200x magnification with patent perforators

| phenox p64 | Competitor A | Competitor B |
|------------|--------------|--------------|
| | | |

Ø 4.0 mm device in Ø 3.75 mm silicon tube; data on file

Excellent visibility due to **helical strands and eight proximal markers**.



Case images by courtesy of Prof. Dr. Pedro Lylyk, Clínica La Sagrada Familia, Buenos Aires, Argentina

