


Elecsys Testosterone II

cobas®

REF			SYSTEM
08946370190	08946370500	300	cobas e 402 cobas e 801

English

System information

Short name	ACN (application code number)
TESTO 2	10020

Intended use

Immunoassay for the in vitro quantitative determination of testosterone in human serum and plasma.

The electrochemiluminescence immunoassay "ECLIA" is intended for use on cobas e immunoassay analyzers.

Summary

Testosterone is regarded as one of the key androgen steroids. It is a steroid secreted from the testis and the adrenal cortex in men and from the adrenal cortex and the ovary in women. It is also produced by the peripheral tissues from androstenedione.

In men, testosterone is synthesized almost exclusively by the Leydig cells of the testes. The secretion of testosterone is regulated by luteinizing hormone (LH) and testosterone promotes the development of the secondary sex characteristics, such as the growth of pubic, facial, and axillary hair, or the accessory sex organs. Most of the circulating testosterone is bound to carrier proteins (SHBG = sex hormone-binding globulin).^{1,2,3}

In women, small quantities of testosterone are formed in the ovaries, adrenal gland, and peripheral fatty tissues, and it has a serum concentration that is approximately 10 times less than in males. In physiological concentrations, androgens have no specific effects in women. Increased production of testosterone in women can cause virilization (depending on the increase).^{2,3}

The Elecsys Testosterone II assay is based on a competitive test principle using a high affinity monoclonal antibody (sheep) specifically directed against testosterone. Endogenous testosterone released from the sample by 2-bromoestradiol competes with the added testosterone derivative labeled with a ruthenium complex^{a)} for the binding sites on the biotinylated antibody.

a) Tris(2,2'-bipyridyl)ruthenium(II)-complex (Ru(bpy)₃²⁺)

Test principle

Competition principle. Total duration of assay: 18 minutes.

- 1st incubation: 12 µL of sample are incubated with a biotinylated monoclonal testosterone-specific antibody. The binding sites of the labeled antibody become occupied by the sample analyte (depending on its concentration).
- 2nd incubation: After addition of streptavidin-coated microparticles and a testosterone derivative labeled with a ruthenium complex, the complex becomes bound to the solid phase via interaction of biotin and streptavidin.
- The reaction mixture is aspirated into the measuring cell where the microparticles are magnetically captured onto the surface of the electrode. Unbound substances are then removed with ProCell II M. Application of a voltage to the electrode then induces chemiluminescent emission which is measured by a photomultiplier.
- Results are determined via a calibration curve which is instrument-specifically generated by 2-point calibration and a master curve provided via the cobas link.

Reagents - working solutions

The cobas e pack is labeled as TESTO 2.

- M Streptavidin-coated microparticles, 1 bottle, 12.4 mL:
Streptavidin-coated microparticles 0.72 mg/mL, preservative.

- R1 Anti-testosterone-Ab~biotin, 1 bottle, 21.0 mL:
Biotinylated monoclonal anti-testosterone antibody (sheep) 40 ng/mL; releasing reagent 2-bromoestradiol; MES^{b)} buffer 50 mmol/L, pH 6.0; preservative.

- R2 Testosterone-peptide~Ru(bpy)₃²⁺, 1 bottle, 18.8 mL:
Testosterone derivative, labeled with ruthenium complex 1.5 ng/mL; MES buffer 50 mmol/L, pH 6.0; preservative.

b) MES = 2-morpholino-ethane sulfonic acid

Precautions and warnings

For in vitro diagnostic use for health care professionals. Exercise the normal precautions required for handling all laboratory reagents.

Infectious or microbial waste:

Warning: handle waste as potentially biohazardous material. Dispose of waste according to accepted laboratory instructions and procedures.

Environmental hazards:

Apply all relevant local disposal regulations to determine the safe disposal.

Safety data sheet available for professional user on request.

This kit contains components classified as follows in accordance with the Regulation (EC) No. 1272/2008:



Warning

- H317 May cause an allergic skin reaction.

Prevention:

- P261 Avoid breathing dust/fume/gas/mist/vapours/spray.
- P272 Contaminated work clothing should not be allowed out of the workplace.
- P280 Wear protective gloves.

Response:

- P333 + P313 If skin irritation or rash occurs: Get medical advice/attention.
- P362 + P364 Take off contaminated clothing and wash it before reuse.

Disposal:

- P501 Dispose of contents/container to an approved waste disposal plant.

Product safety labeling follows EU GHS guidance.

Contact phone: all countries: +49-621-7590

Avoid foam formation in all reagents and sample types (specimens, calibrators and controls).

Reagent handling

The reagents in the kit have been assembled into a ready-for-use unit that cannot be separated.

All information required for correct operation is available via the cobas link.

Storage and stability

Store at 2-8 °C.

Do not freeze.

Store the cobas e pack **upright** in order to ensure complete availability of the microparticles during automatic mixing prior to use.

Elecsys Testosterone II

Stability:	
unopened at 2-8 °C	up to the stated expiration date
on the analyzers	16 weeks

Specimen collection and preparation

Only the specimens listed below were tested and found acceptable.

Serum collected using standard sampling tubes or tubes containing separating gel.

Li-heparin, K₂-EDTA and K₃-EDTA plasma.

Criterion: Recovery within 80-120 % of serum value > 1 ng/mL, recovery of ± 0.2 ng/mL of serum value ≤ 1 ng/mL and slope 0.9-1.1 + bias at 0.5 ng/mL and 3.0 ng/mL ≤ 10 % + coefficient of correlation ≥ 0.95 .

Stable for 14 days at 2-8 °C, 5 days at 20-25 °C, 6 months at -20 °C (± 5 °C). Freeze only once.

The sample types listed were tested with a selection of sample collection tubes that were commercially available at the time of testing, i.e. not all available tubes of all manufacturers were tested. Sample collection systems from various manufacturers may contain differing materials which could affect the test results in some cases. When processing samples in primary tubes (sample collection systems), follow the instructions of the tube manufacturer.

Centrifuge samples containing precipitates before performing the assay.

Do not use heat-inactivated samples.

Do not use samples and controls stabilized with azide.

Ensure the samples and calibrators are at 20-25 °C prior to measurement.

Due to possible evaporation effects, samples and calibrators on the analyzers should be analyzed/measured within 2 hours.

Materials provided

See "Reagents – working solutions" section for reagents.

Materials required (but not provided)

- REF 05202230190, Testosterone II CalSet II, for 4 x 1.0 mL
- REF 11731416190, PreciControl Universal, for 4 x 3.0 mL
- General laboratory equipment
- cobas e** analyzer

Additional materials for **cobas e** 402 and **cobas e** 801 analyzers:

- REF 06908799190, ProCell II M, 2 x 2 L system solution
- REF 04880293190, CleanCell M, 2 x 2 L measuring cell cleaning solution
- REF 07485409001, Reservoir Cup, 8 cups to supply ProCell II M and CleanCell M
- REF 06908853190, PreClean II M, 2 x 2 L wash solution
- REF 05694302001, Assay Tip/Assay Cup tray, 6 magazines x 6 magazine stacks x 105 assay tips and 105 assay cups, 3 wasteliners
- REF 07485425001, Liquid Flow Cleaning Cup, 2 adaptor cups to supply ISE Cleaning Solution/Elecsys SysClean for Liquid Flow Cleaning Detection Unit
- REF 07485433001, PreWash Liquid Flow Cleaning Cup, 1 adaptor cup to supply ISE Cleaning Solution/Elecsys SysClean for Liquid Flow Cleaning PreWash Unit
- REF 11298500316, ISE Cleaning Solution/Elecsys SysClean, 5 x 100 mL system cleaning solution

Assay

For optimum performance of the assay follow the directions given in this document for the analyzer concerned. Refer to the appropriate operator's manual for analyzer-specific assay instructions.

Resuspension of the microparticles takes place automatically prior to use.

Place the cooled (stored at 2-8 °C) **cobas e** pack on the reagent manager. Avoid foam formation. The system automatically regulates the temperature of the reagents and the opening/closing of the **cobas e** pack.

Calibration

Traceability: This method is traceable to highly purified testosterone by weight via ID-GC/MS ("Isotope Dilution - Gas Chromatography/Mass Spectrometry").⁴

The predefined master curve is adapted to the analyzer using the relevant CalSet.

Calibration frequency: Calibration must be performed once per reagent lot using fresh reagent (i.e. not more than 24 hours since the **cobas e** pack was registered on the analyzer).

Calibration interval may be extended based on acceptable verification of calibration by the laboratory.

Renewed calibration is recommended as follows:

- after 12 weeks when using the same reagent lot
- after 28 days when using the same **cobas e** pack on the analyzer
- as required: e.g. quality control findings outside the defined limits

Quality control

For quality control, use PreciControl Universal.

In addition, other suitable control material can be used.

Controls for the various concentration ranges should be run individually at least once every 24 hours when the test is in use, once per **cobas e** pack, and following each calibration.

The control intervals and limits should be adapted to each laboratory's individual requirements. Values obtained should fall within the defined limits. Each laboratory should establish corrective measures to be taken if values fall outside the defined limits.

If necessary, repeat the measurement of the samples concerned.

Follow the applicable government regulations and local guidelines for quality control.

Calculation

The analyzer automatically calculates the analyte concentration of each sample (either in ng/mL, ng/dL or nmol/L).

Conversion factors:	ng/mL x 3.47 = nmol/L
	ng/mL x 100 = ng/dL
	nmol/L x 0.288 = ng/mL

Limitations - interference

The effect of the following endogenous substances and pharmaceutical compounds on assay performance was tested. Interferences were tested up to the listed concentrations and no impact on results was observed.

Endogenous substances

Compound	Concentration tested
Bilirubin	≤ 513 μ mol/L or ≤ 30 mg/dL
Hemoglobin	≤ 0.373 mmol/L or ≤ 600 mg/dL
Intralipid	≤ 800 mg/dL
Biotin	≤ 3600 ng/mL
Rheumatoid factors	≤ 1000 IU/mL

Criterion: Recovery within ± 10 % of initial value (concentration range > 1-15 ng/mL), recovery within ± 15 % of initial value (concentration range > 0.5-1 ng/mL) and recovery of ± 0.075 ng/mL (concentration range of 0.025-0.500 ng/mL).

Pharmaceutical substances

In vitro tests were performed on 17 commonly used pharmaceuticals and 2 special pharmaceuticals. Of these, only phenylbutazone at therapeutic dosage levels showed interference with the assay (testosterone values increased).

A strong interaction with Nandrolone (INN international nonproprietary name, WHO) was found. Do not use samples from patients under Nandrolone treatment.

Testosterone undecanoate (INN international nonproprietary name, WHO) is metabolized to testosterone after administration. The Elecsys Testosterone II assay does not differentiate between endogenous

Elecsys Testosterone II

testosterone and exogenous testosterone resulting from metabolized testosterone under testosterone supplementation therapy.

In isolated cases, elevated testosterone levels can be seen in samples from female patients with end stage renal disease (ESRD).

Implausible elevated testosterone values in women should be verified by an extraction method or a validated LC-MS/MS tandem method.⁵

In rare cases, interference due to extremely high titers of antibodies to analyte-specific antibodies, streptavidin or ruthenium can occur. These effects are minimized by suitable test design.

For diagnostic purposes, the results should always be assessed in conjunction with the patient's medical history, clinical examination and other findings.

Limits and ranges

Measuring range

0.025-15.0 ng/mL or 0.087-52.0 nmol/L (defined by the Limit of Detection and the maximum of the master curve). Values below the Limit of Detection are reported as < 0.025 ng/mL or < 0.087 nmol/L. Values above the measuring range are reported as > 15.0 ng/mL or > 52.0 nmol/L.

Lower limits of measurement

Limit of Blank, Limit of Detection and Limit of Quantitation

Limit of Blank = 0.015 ng/mL (0.052 nmol/L)

Limit of Detection = 0.025 ng/mL (0.087 nmol/L)

Limit of Quantitation = 0.120 ng/mL (0.416 nmol/L)

The Limit of Blank, Limit of Detection and Limit of Quantitation were determined in accordance with the CLSI (Clinical and Laboratory Standards Institute) EP17-A2 requirements.

The Limit of Blank is the 95th percentile value from $n \geq 60$ measurements of analyte-free samples over several independent series. The Limit of Blank corresponds to the concentration below which analyte-free samples are found with a probability of 95 %.

The Limit of Detection is determined based on the Limit of Blank and the standard deviation of low concentration samples. The Limit of Detection corresponds to the lowest analyte concentration which can be detected (value above the Limit of Blank with a probability of 95 %).

The Limit of Quantitation is defined as the lowest amount of analyte in a sample that can be accurately quantitated with a total allowable relative error of ≤ 20 %.

Dilution

Not necessary due to the broad measuring range.

Expected values

The following tables show the results obtained using the Elecsys Testosterone II assay in a reference population of 95 males (7-18 years) and 100 females (8-18 years), who were in good endocrinological health. Subjects were clinically characterized according to their Tanner Stage. Tanner Stage was characterized according to the method of Marshall and Tanner.^{6,7}

Reference values for males (7-18 years) characterized by Tanner Stage

Tanner Stage	N	Median	5-95 th percentiles (ng/mL)
1	26	< 0.025	< 0.025
2	18	0.597	< 0.025-4.32
3	15	2.45	0.649-7.78
4	16	3.44	1.80-7.63
5	20	4.46	1.88-8.82

Reference values for females (8-18 years) characterized by Tanner Stage

Tanner Stage	N	Median	5-95 th percentiles (ng/mL)
1	37	< 0.025	< 0.025-0.061
2	12	< 0.025	< 0.025-0.104
3	12	0.079	< 0.025-0.237
4	12	0.122	< 0.025-0.268

Tanner Stage	N	Median	5-95 th percentiles (ng/mL)
5	27	0.197	0.046-0.383

The following table shows the results obtained with the Elecsys Testosterone II assay in an apparently healthy group of 214 males and 160 females without intake of contraceptives and prescription drugs (study number CIM 000669). Blood samples were taken between 6.30 am and 1.00 pm. This clinical study with focus on the Elecsys Testosterone II assay included measurements in parallel with the Elecsys SHBG assay. The results were evaluated for the Elecsys Testosterone II and Elecsys SHBG assays and commonly used parameters derived from different calculation procedures, including albumin as an important parameter involved.⁸

- Free testosterone index (% FTI) or free androgen index (% FAI) as calculated on a molar/molar basis:


$$\text{FTI (\%)} = (\text{testosterone in nmol/L divided by SHBG in nmol/L}) \times 100$$
 - Free testosterone calculated (FTc) in nmol/L and %
 - Bioavailable testosterone calculated (BATc) in nmol/L and %
- FTc and BATc were calculated by means of individual concentrations for total testosterone, SHBG, and albumin and via the association constant of albumin to testosterone. A detailed description of the calculation procedure is available on request. Refer also to the homepage of www.issam.ch/freetesto.htm.

The following results were obtained:

Testosterone

Test subjects	Percentiles				
	N	Median	5-95 th	Median	5-95 th
		ng/mL		nmol/L	
Males	136	5.36	2.49-8.36	18.6	8.64-29.0
20-49 years					
Males	78	4.76	1.93-7.40	16.5	6.68-25.7
≥ 50 years					
Females	89	0.271	0.084-0.481	0.941	0.290-1.67
20-49 years					
Females	71	0.162	0.029-0.408	0.563	0.101-1.42
≥ 50 years					

Distribution of testosterone values in the apparently healthy male group based on age ($n = 214$). Solid line: 50 % percentile, upper line: 95 % percentile, lower line: 5 % percentile.

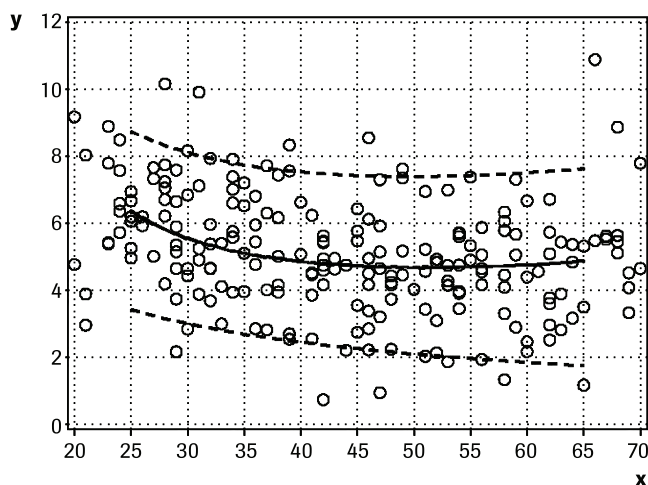


x: Age (years)

y: Testosterone (ng/mL) - male group

Elecsys Testosterone II

Distribution of testosterone values in the apparently healthy female group based on age (n = 160). Solid line: 50 % percentile, upper line: 95 % percentile, lower line: 5 % percentile.

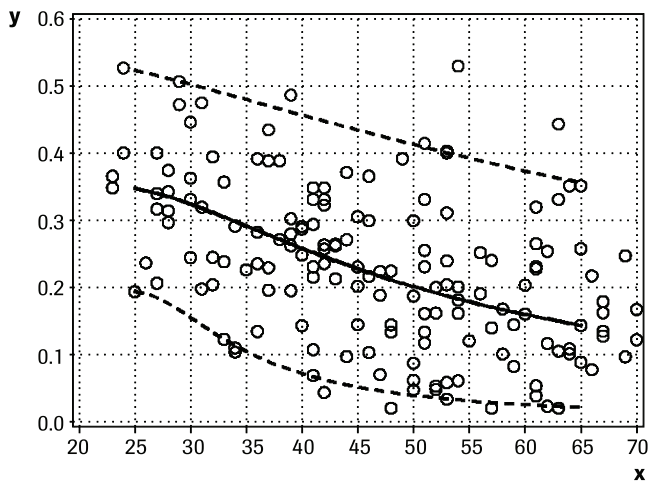

x: Age (years)

y: Testosterone (ng/mL) - female group

SHBG

Test subjects	N	Median	5-95 th percentiles
		nmol/L	
Males 20-49 years	136	33.5	16.5-55.9
Males ≥ 50 years	78	40.8	19.3-76.4
Females 20-49 years	89	64.3	24.6-122
Females ≥ 50 years	71	57.4	17.3-125

Free testosterone index or free androgen index

Test subjects	N	Median	5-95 th percentiles
		FTI or FAI (%)	
Males 20-49 years	136	57.2	35.0-92.6
Males ≥ 50 years	78	38.2	24.3-72.1
Females 20-49 years	89	1.53	0.297-5.62
Females ≥ 50 years	71	1.15	0.187-3.63

Free testosterone, calculated

Test subjects	N	Percentiles			
		Median	5-95 th percentiles	Median	5-95 th percentiles
		FTc (nmol/L)		FTc (%)	
Males 20-49 years	136	0.379	0.198-0.619	2.10	1.53-2.88
Males ≥ 50 years	78	0.304	0.163-0.473	1.91	1.23-2.59
Females 20-49 years	89	0.011	0.003-0.033	1.19	0.701-2.19
Females ≥ 50 years	71	0.008	0.001-0.020	1.26	0.685-2.64

Bioavailable testosterone, calculated

Test subjects	N	Percentiles			
		Median	5-95 th percentiles	Median	5-95 th percentiles
		BATc (nmol/L)		BATc (%)	
Males 20-49 years	136	9.10	4.36-14.3	49.8	35.0-66.3
Males ≥ 50 years	78	6.63	3.59-11.0	42.1	27.5-60.7
Females 20-49 years	89	0.246	0.059-0.756	25.7	15.3-47.7
Females ≥ 50 years	71	0.168	0.030-0.430	28.0	15.1-55.2

Each laboratory should investigate the transferability of the expected values to its own patient population and if necessary determine its own reference ranges.

Specific performance data

Representative performance data on the analyzers are given below. Results obtained in individual laboratories may differ.

Precision

Precision was determined using Elecsys reagents, pooled human sera and controls in a protocol (EP05-A3) of the CLSI (Clinical and Laboratory Standards Institute): 2 runs per day in duplicate each for 21 days (n = 84). The following results were obtained:

cobas e 402 and cobas e 801 analyzers					
Sample	Mean		Repeatability		
	ng/mL	nmol/L	SD	CV	
Human serum 1	0.100	0.347	0.006	0.020	5.7
Human serum 2	0.315	1.09	0.009	0.032	3.0
Human serum 3	0.765	2.65	0.012	0.043	1.6
Human serum 4	2.09	7.25	0.032	0.111	1.5
Human serum 5	13.9	48.2	0.235	0.815	1.7
PC ^{c)} Universal 1	5.58	19.4	0.071	0.246	1.3
PC Universal 2	2.57	8.92	0.035	0.120	1.3

c) PC = PreciControl

cobas e 402 and cobas e 801 analyzers					
Sample	Mean		Intermediate precision		
	Mean		SD		
	ng/mL	nmol/L	ng/mL	nmol/L	%
Human serum 1	0.100	0.347	0.012	0.040	11.5
Human serum 2	0.315	1.09	0.015	0.051	4.7
Human serum 3	0.765	2.65	0.025	0.086	3.2
Human serum 4	2.09	7.25	0.046	0.161	2.2
Human serum 5	13.9	48.2	0.306	1.06	2.2
PC Universal 1	5.58	19.4	0.112	0.389	2.0
PC Universal 2	2.57	8.92	0.051	0.177	2.0

Method comparison

a) A comparison of the Elecsys Testosterone II assay, [REF] 08946370190 (cobas e 402 analyzer; y) with the Elecsys Testosterone II assay, [REF] 08946370190 (cobas e 801 analyzer; x) gave the following correlations (ng/mL):

Elecsys Testosterone II

Number of samples measured: 166

Passing/Bablok⁹ Linear regression

$y = 1.02x - 0.006$ $y = 1.02x - 0.003$

$r = 0.984$ $r = 0.999$

The sample concentrations were between 0.029 and 14.2 ng/mL.

b) A comparison of the Elecsys Testosterone II assay, [REF] 08946370190 (cobas e 801 analyzer; y) with the Elecsys Testosterone II assay, [REF] 07027915190 (cobas e 801 analyzer; x) gave the following correlations (ng/mL):

Number of samples measured: 169

Passing/Bablok⁹ Linear regression

$y = 1.02x - 0.027$ $y = 1.02x - 0.060$

$r = 0.980$ $r = 0.999$

The sample concentrations were between 0.046 and 14.0 ng/mL.

c) A comparison of the Elecsys Testosterone II assay, [REF] 08946370190 (cobas e 801 analyzer; y) with the Elecsys Testosterone II assay, [REF] 08946370190 (cobas e 601 analyzer; x) gave the following correlations (ng/mL):

Number of samples measured: 167

Passing/Bablok⁹ Linear regression

$y = 0.999x - 0.039$ $y = 0.978x + 0.040$

$r = 0.979$ $r = 0.998$

The sample concentrations were between 0.040 and 14.4 ng/mL.

Analytical specificity

For the antibody derivative used, the following cross-reactivities were found (in %):

	Concentration ng/mL	Cross-reactivity %
Androstendione	100	2.66
Cortisol	1000	0.016
Cortisone	2000	0.002
Danazol	1000	0.442
Dexamethasone	2000	0.0004
DHEA	1000	0.007
DHEA-S	50000	0.001
D-5-Androstene-3 β ,17 β -diol	1000	0.186
Estradiol	1000	0.148
Estrone	1000	n.d. ^{d)}
Ethisterone	1000	2.78
Norgestrel	1000	0.461
Testosterone propionate	100	3.73
5- α -Androstane-3 β ,17 β -diol	1000	3.65
5- α -Dihydro-testosterone	500	1.84
11- β -Hydroxy-testosterone	100	20.4
11-Keto-testosterone	1000	3.79
19-Norethisterone	40	3.44
Prednisone	1000	0.004
Prednisolone	1000	0.016
Progesterone	1000	0.023

d) n.d. = not detectable

References

- 1 Wilson JD, Foster DW (Eds). Williams Textbook of Endocrinology. 8th Edition, W.B. Saunders, Philadelphia, Pennsylvania 19106, 1992: 822-832.
- 2 Brutis CA, Ashwood ER (Eds). Tietz Fundamentals of Clinical Chemistry, 4th Edition W.B. Saunders, Philadelphia, Pennsylvania 19106, 1996: 671 - 672.
- 3 Wheeler MJ. The determination of bio-available testosterone. Ann Clin Biochem 1995;32:345-357.
- 4 Thienpont LM, De Brabandere VI, Stöckl D, et al. Use of cyclodextrins for prepurification of progesterone and testosterone from human serum prior to determination with isotope dilution-gas chromatography/mass spectrometry. Anal Chem 1994;66:4116-4119.
- 5 Rosner W, Auchus RJ, Azzis R, et al. Position Statement: Utility, Limitations, and Pitfalls in Measuring Testosterone: An Endocrine Society Positions Statement. J Clin Endocrinol Metab 2007;92(2):404-413.
- 6 Marshall WA, Tanner JM. Variations in the pattern of pubertal changes in boys. Arch Dis Childh 1970;45:13-23.
- 7 Marshall WA, Tanner JM. Variations in the pattern of pubertal changes in girls. Arch Dis Childh 1969;44:291-303.
- 8 Vermeulen A, Verdonck L, Kaufman JM. A critical evaluation of simple methods for the estimation of free testosterone in serum. J Clin Endocrinol Metab 1999;84:3666-3672.
- 9 Bablok W, Passing H, Bender R, et al. A general regression procedure for method transformation. Application of linear regression procedures for method comparison studies in clinical chemistry, Part III. J Clin Chem Clin Biochem 1988 Nov;26(11):783-790.

For further information, please refer to the appropriate operator's manual for the analyzer concerned, the respective application sheets, the product information and the Method Sheets of all necessary components (if available in your country).

A point (period/stop) is always used in this Method Sheet as the decimal separator to mark the border between the integral and the fractional parts of a decimal numeral. Separators for thousands are not used.

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the Member State in which the user and/or the patient is established.

Symbols

Roche Diagnostics uses the following symbols and signs in addition to those listed in the ISO 15223-1 standard (for USA: see dialog.roche.com for definition of symbols used):

CONTENT	Contents of kit
SYSTEM	Analyzers/Instruments on which reagents can be used
REAGENT	Reagent
CALIBRATOR	Calibrator
→	Volume after reconstitution or mixing
GTIN	Global Trade Item Number

COBAS, COBAS E, ELECSYS and PRECICONTROL are trademarks of Roche. INTRALIPID is a trademark of Fresenius Kabi AB.

All other product names and trademarks are the property of their respective owners.

Additions, deletions or changes are indicated by a change bar in the margin.

© 2020, Roche Diagnostics



Roche Diagnostics GmbH, Sandhofer Strasse 116, D-68305 Mannheim
www.roche.com
+800 5505 6606

