

AMPLATZER PICCOLO™ OCCLUDER

**CLOSES EARLY PDAs.  
FILLS LOVING HEARTS.**

**PROVEN PDA CLOSURE  
FOR PATIENTS 700G AND UP.**

Information contained herein for **DISTRIBUTION in Europe, Middle East and Africa ONLY.**  
Check the regulatory status of the device in areas where CE marking is not the regulation in force.





**A NEW LEVEL OF VERSATILITY AND  
PROVEN SAFETY FOR THE YOUNGEST  
INFANTS AND UP.**

**BUILT ON THE EXTENSIVE AMPLATZER™ LEGACY  
OF SAFETY AND EFFICACY**


- Pioneered transcatheter occlusion
- Over 1.25 million devices implanted worldwide<sup>1</sup>
- More than 20 years of clinical experience

Information contained herein for **DISTRIBUTION in Europe, Middle East and Africa ONLY**.  
Check the regulatory status of the device in areas where CE marking is not the regulation in force.

# CLINICALLY PROVEN OUTCOMES.

A recent study using the Amplatzer Piccolo™ Occluder for PDA closure demonstrated safety and effectiveness with a low rate of major complications and a high rate of PDA closure.

## STUDY HIGHLIGHTS




### IMPLANT SUCCESS

100% for patients ≤ 2kg  
87.5% for patients >2kg



### EFFECTIVE CLOSURE\*

At 6 months



### MAJOR COMPLICATIONS\*\*

Through 180 days

TOTAL NUMBER OF PATIENTS: 50		≤ 2 kg (N=18)	> 2 kg (N=32)
DEMOGRAPHICS			
<b>Age, Months</b>			
Mean ± SD		1.23 ± 0.55	24.88 ± 38.17
Range		(0.49 - 2.30)	(0.66 - 168.54)
<b>Weight (kg)</b>			
Mean ± SD		1.34 ± 0.38	10.29 ± 10.42
Range		(0.76 - 1.90)	(2.03 - 47.80)
PDA CHARACTERISTICS (by echocardiography)			
<b>Minimal PDA Diameter (mm)</b>			
Mean ± SD		2.72 ± 0.65	2.64 ± 0.58
Range		(1.4 - 4.0)	(1.5 - 4.0)
<b>PDA Length (mm)</b>			
Mean ± SD		8.81 ± 2.55	7.98 ± 2.78
Range		(4.6 - 14.0)	(3.1 - 16.0)
PROCEDURE CHARACTERISTICS			
<b>Implant Success (%)</b>		100.0% (18/18)	87.5% (28/32)
<b>Fluoroscopy Time (min)</b>			
Mean ± SD		9.8 ± 4.9	10.9 ± 8.5
Range		(4 - 22)	(5 - 43)
<b>Anterograde Implant</b>		100.0% (18/18)	64.3% (18/28)
<b>Femoral Arterial Access</b>		0.0% (0/18)	46.9% (15/32)
<b>In NICU at time of baseline assessment</b>		100.0% (18/18)	21.9% (7/32)
OUTCOMES			
Major complications rate (%)**		0% (0/18)	0% (0/32)
Effective closure at 6 months (Echo Core Lab Assessed) (%)***		100% (17/17)	100% (27/27)
Effective closure at 6 months (Site Assessed) (%)		100% (18/18)	100% (28/28)

\*Assessed by echocardiography and defined as the presence of either a grade 0 (none) or grade 1 (trivial) shunt.

\*\*Major complications were defined as "device or procedure-related adverse events resulting in death, life-threatening adverse event, persistent or significant disability and/or surgical intervention."

\*\*\*The core lab was unable to determine shunt grade in two subjects due to incomplete imaging views.

# ADVANCING A PROVEN PLATFORM FOR PREDICTABLE RESULTS.

As the only PDA closure solution indicated for premature infants ( $\geq 700\text{g}$  +  $\geq 3$  days old) and proven to deliver safe and effective closure, Amplatzer Piccolo™ Occluder offers new opportunities to care for a wider range of patients than ever before.

## RELIABILITY BY DESIGN.

### TIGHTLY WOVEN SINGLE-LAYER MESH


Designed to minimize residual shunt immediately after placement

### ENGINEERED FOR STRUCTURE AND STRENGTH

Occludes ducts while minimizing protrusion into surrounding vasculature

### INTAGLIO WIRE TREATMENT

Designed to reduce nickel leaching

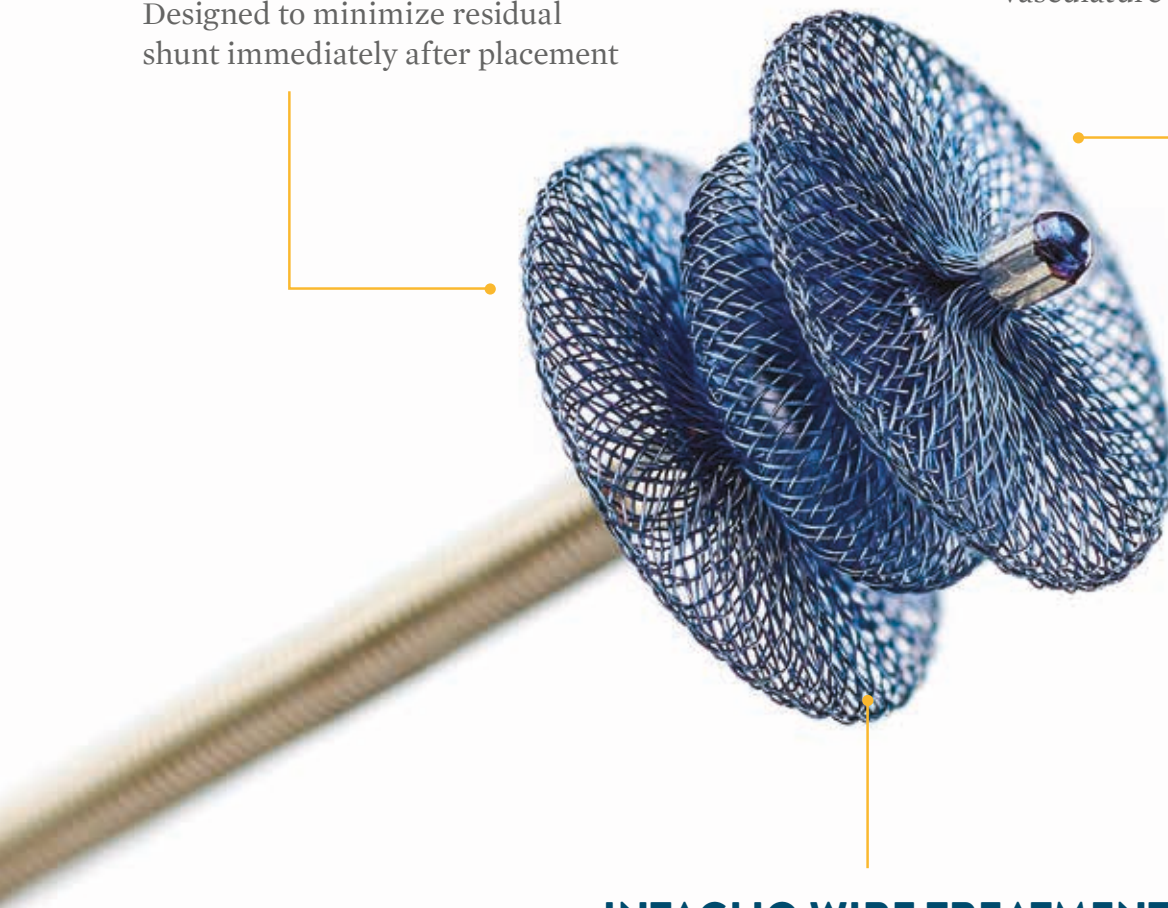


## SMOOTH DELIVERY IN EVEN THE MOST CHALLENGING MORPHOLOGIES.

### PREDICTABLE PLACEMENT

Disc size and shape designed for predictable positioning in the duct

### DELIVERABLE IN 4 FRENCH SYSTEM

4 F catheter facilitates delivery in small vasculatures



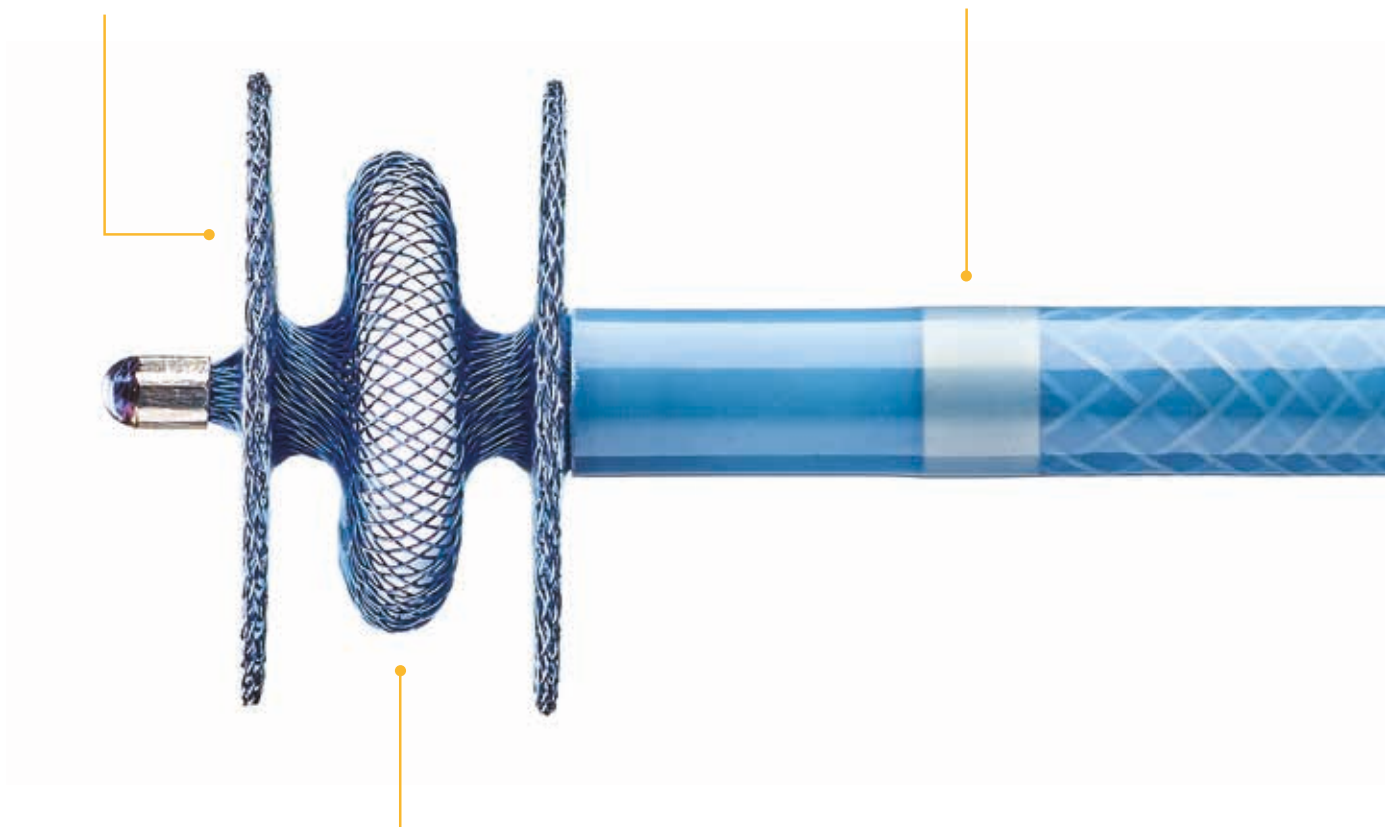














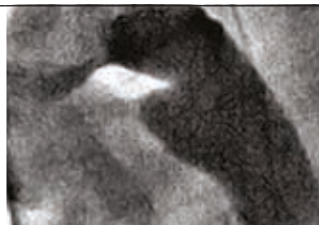


### PROCEDURAL FLEXIBILITY

Symmetrical design offers procedural flexibility to choose an antegrade (venous) or retrograde (arterial) approach. For infants  $\leq 2\text{kg}$ , a venous approach is recommended.

# THE RIGHT CHOICE FOR A WIDE RANGE OF

The versatile design and predictable performance of the Amplatzer Piccolo™ Occluder make it ideal for a variety of morphologies. From “conical” ductus to “fetal type” ductus, the Piccolo device has you covered.

PDA TYPE DESCRIPTION <sup>2</sup>		PDA <sup>2</sup>	DEVICE CLOSURE <sup>2</sup>
<b>TYPE A:</b> <b>“Conical” ductus</b> , with well defined aortic ampulla and constricted pulmonary artery end.			
<b>TYPE B:</b> <b>“Window” ductus</b> , with short length, slightly constricted aortic end and wide pulmonary artery end.			
<b>TYPE C:</b> <b>“Tubular” ductus</b> , without any constrictions at the aortic end or the pulmonary artery end.			
<b>TYPE D:</b> <b>“Saccular” ductus</b> , with constricted aortic end and pulmonary artery end with a wide center.			
<b>TYPE E:</b> <b>“Elongated” ductus</b> , which is narrow with a constricted pulmonary artery end.			
<b>TYPE F:</b> <b>“Fetal Type” ductus</b> , found exclusively in children born prematurely and is long, wide and tortuous.			

Information contained herein for **DISTRIBUTION in Europe, Middle East and Africa ONLY**.  
 Check the regulatory status of the device in areas where CE marking is not the regulation in force.

# F ANATOMIES.

PRE-TERM <sup>2</sup>	FULL TERM <sup>2</sup>
6%	40%
—	2%
—	10%
6%	5%
9%	43%
79%	—

## EXPERT SUPPORT AT EVERY TURN.

### CLINICAL CASE SUPPORT

- Experienced field personnel
- Over two decades of excellence

### CLINICAL TRAINING PROGRAMS

- Training centers and online courses
- Fellows programs

# AMPLATZER PICCOLO™ OCCLUDER

## Device Specifications


SIZING AND DEVICE SELECTION				
Model/Reorder Number	Waist Diameter (mm) [A]	Length between discs (mm) [B]	Disc Diameter (mm) [C]	Recommended Sheath Size
9-PDAP-03-02-L	3 mm	2 mm	4.00	4 F; 90° Curve
9-PDAP-03-04-L	3 mm	4 mm	4.00	4 F; 90° Curve
9-PDAP-03-06-L	3 mm	6 mm	4.00	4 F; 90° Curve
9-PDAP-04-02-L	4 mm	2 mm	5.25	4 F; 90° Curve
9-PDAP-04-04-L	4 mm	4 mm	5.25	4 F; 90° Curve
9-PDAP-04-06-L	4 mm	6 mm	5.25	4 F; 90° Curve
9-PDAP-05-02-L	5 mm	2 mm	6.50	4 F; 90° Curve
9-PDAP-05-04-L	5 mm	4 mm	6.50	4 F; 90° Curve
9-PDAP-05-06-L	5 mm	6 mm	6.50	4 F; 90° Curve

### T1 Dimensions

[A] Waist diameter

[B] Length between retention discs

[C] Retention disc diameter



For more information about the Amplatzer Piccolo™ Occluder,  
contact your Abbott sales representative  
or visit [INFANTPDA.COM](http://INFANTPDA.COM).

### References

1. Data on file at Abbott. 2. Philip, R., Rush Waller, B., Agrawal, V., Wright, D., Arevalo, A., Zurakowski, D. and Sathanandam, S. (2016), Morphologic characterization of the patent ductus arteriosus in the premature infant and the choice of transcatheter occlusion device. *Cathet. Cardiovasc. Intervent.*, 87: 310–317.

**CAUTION:** This product is intended for use by or under the direction of a physician. Prior to use, reference the Instructions for Use, inside the product carton (when available) or at [eifu.abbottvascular.com](http://eifu.abbottvascular.com) or at [medical.abbott/manuals](http://medical.abbott/manuals) for more detailed information on Indications, Contraindications, Warnings, Precautions and Adverse Events.

Information contained herein for **DISTRIBUTION in Europe, Middle East and Africa ONLY**.

Check the regulatory status of the device in areas where CE marking is not the regulation in force.

Illustrations are artist's representations only and should not be considered as engineering drawings or photographs.

Photo(s) on file at Abbott.

**Abbott Vascular International BVBA**

Park Lake, Culliganlaan 2b, 1831 Diegem, Belgium

[www.cardiovascular.abbott](http://www.cardiovascular.abbott)

™ Indicates a trademark of the Abbott group of companies.

‡ Indicates a third party trademark, which is property of its respective owner.

© 2019 Abbott. All Rights Reserved. SJM-AMPL-0119-0148(1)a | 9-EH-1-9942-01 07-2019

