




**Product Specification**  
**Cell culture plate, 96 well, surface: Standard,  
round base**

**Page 1**

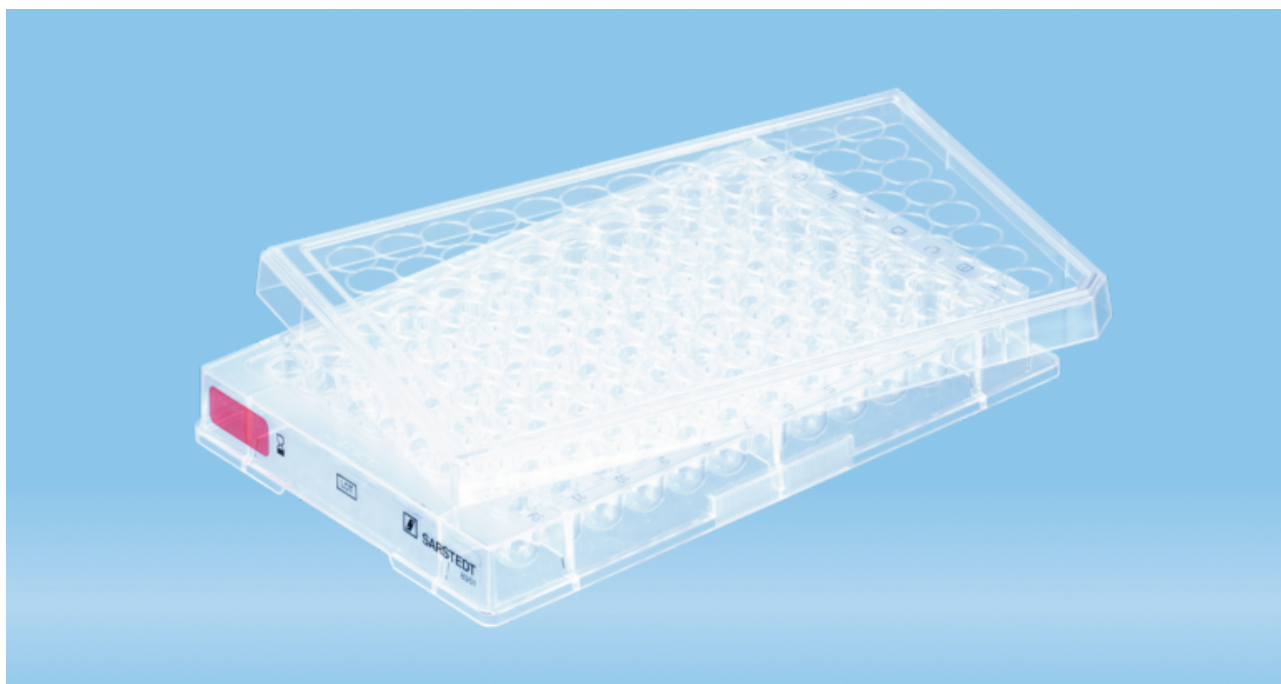

**Product description**

Order number	83.3925
Product description	Cell culture plate, 96 well, material: PS, surface: Standard, for adherent cells, coding colour: red, round base, TC Tested, 1 piece(s)/blister

**Product characteristics**

Label/ Print	with plastic label
Closure type	slip-on lid
Cell type	adherent cells
Base shape	round base
Number of wells	96
Vessel type	Plate
Coding colour	red

This is the current specification for this product. Sarstedt reserves the right to make changes, in full or in part, at any time without prior notification.

This specification is confidential and the property of Sarstedt. It is neither to be duplicated nor made available to third parties without our prior written consent.





**Product Specification**  
**Cell culture plate, 96 well, surface: Standard,  
round base**

**Page 2**

**Size**

Max. volume	0.31 ml
Width of product	85.2 mm
Height of product	16.55 mm
Length of product	127.8 mm

**Material & colours**

Product material	Polystyrene (PS)
Colour of product	transparent
Closure material	Polystyrene (PS)

**Purity & certification**

Product category	no medical device   IVD
Purity standard	TC Tested
Sterilisation	Gamma irradiation
Pyrogen-free	yes
Non-cytotoxic	yes
Batched	yes

**Packaging**

Minimum order qty.	50
Type of smallest subpackaging	blister
Piece(s) / inner box	1
Piece (s) / outer case	50
Piece(s) / pallet	3200
Depth of case	332 mm
Width of case	297 mm
Height of case	215 mm
Case volume	0.0212 cbm
Weight of product	0.0498 kg
Weight of case	3.19 kg
EAN of inner box	4038917338790
EAN case	4038917338783

This is the current specification for this product. Sarstedt reserves the right to make changes, in full or in part, at any time without prior notification.

This specification is confidential and the property of Sarstedt. It is neither to be duplicated nor made available to third parties without our prior written consent.

Date of issue:  
2023-09-18

This document was prepared by EDP support and is valid without signature.



**SARSTEDT**