



MICROSED-SYSTEM®

USER MANUAL



Copyright © 2017 ELITechGroup B.V.

All rights reserved. No part of this document may be reproduced, stored in a retrieval system, or transmitted, in any form or by any means (electronic, mechanical, or otherwise) without the prior written permission of ELITechGroup B.V.

ELITechGroup B.V. reserves the right to modify components of the described instrument at any time, without prior notifications to customers. The contents of this documentation may also be changed without notification.

ELITechGroup B.V. cannot be held responsible for any damage resulting from changes made to the MICROSED-SYSTEM after it was supplied. ELITechGroup B.V. cannot be held responsible for any damage resulting from not complying to the specifications supplied with the MICROSED-SYSTEM.

MICROSED-SYSTEM is a trademark of ELITechGroup B.V. All other trademarks are trademarks or registered trademarks of their respective owners.

ELITechGroup B.V. is also trading as ELITechGroup Clinical Systems.

INSTRUMENT NAME

MICROSED-SYSTEM
ESR Automated Analyzer
10 measuring channels

INSTRUMENT PART NUMBERS

PRD-MSS-EL-08TKNE
PRD-MSS-EL-09TKNE

INSTRUMENT MANUFACTURER



ELITechGroup B.V.
Van Rensselaerweg 4
6956 AV Spankeren
The Netherlands

Tel. +31 313 430 500
service.ecsnl@elitechgroup.com
www.elitechgroup.com



CONTENTS

| | |
|---|----|
| 1. INTRODUCTION | 5 |
| 1.1 Intended use..... | 5 |
| 1.2 Improper use | 5 |
| 2. SAFETY PRECAUTIONS AND POTENTIAL HAZARDS..... | 6 |
| 2.1 Electrical equipment..... | 6 |
| 2.2 Mechanical equipment..... | 6 |
| 2.3 Samples | 6 |
| 2.3.1 Notes on safety measures | 6 |
| 2.4 User precautions | 6 |
| 2.5 Residual risks | 6 |
| 3. DISPOSAL AND RECYCLING | 8 |
| 4. INSTALLATION | 9 |
| 4.1 System description | 9 |
| 4.1.1 Power supply | 9 |
| 4.1.2 Display | 9 |
| 4.1.3 Reading plate..... | 9 |
| 4.1.4 Bar code reader (optional) | 9 |
| 4.1.5 Printer (optional)..... | 10 |
| 4.1.6 Test tubes | 10 |
| 4.1.6.1 Tubes handling requirements | 10 |
| 4.1.6.2 Tubes storage requirements | 10 |
| 4.2 RS232 connector description and I/O data format | 10 |
| 5. MICROSED-SYSTEM START UP..... | 12 |
| 5.1 Positioning of the analyzer | 12 |
| 5.2 Instrument startup | 12 |
| 5.3 Dip-switch configuration | 13 |
| 6. METHODS | 15 |
| 6.1 Westergren method | 15 |
| 6.1.1 Normal ESR values according to Westergren..... | 15 |
| 6.2 Variation of ESR | 15 |
| 7. OPERATING PROCEDURE..... | 17 |
| 7.1 Samples | 17 |
| 7.1.1 Sample collection | 17 |

| | | |
|-------|---|----|
| 7.1.2 | Sample mixing | 17 |
| 7.1.3 | Sample insertion..... | 17 |
| 7.1.4 | Sample identification..... | 17 |
| 7.1.5 | Sample removal..... | 18 |
| 7.2 | Tubes labeling..... | 18 |
| 7.3 | Analysis..... | 19 |
| 7.3.1 | Remaining time..... | 19 |
| 7.3.2 | Results pre-indication..... | 19 |
| 7.4 | Calibration procedures..... | 19 |
| 7.4.1 | Instrument calibration..... | 19 |
| 7.4.2 | Temperature correction | 19 |
| 7.5 | Errors and warnings..... | 20 |
| 7.5.1 | Warnings information | 20 |
| 7.5.2 | System error warnings..... | 20 |
| 7.5.3 | Service | 20 |
| 8. | INTERNAL QUALITY CONTROL..... | 21 |
| 9. | PERFORMANCE CRITERIA AND LIMITATIONS..... | 22 |
| 9.1 | Performance criteria | 22 |
| 9.2 | Limitations..... | 22 |
| 10. | MAINTENANCE | 23 |
| 10.1 | Cleaning instructions | 23 |
| 11. | TROUBLESHOOTING GUIDE..... | 24 |
| 12. | TECHNICAL SPECIFICATIONS..... | 25 |
| 13. | BIBLIOGRAPHY..... | 26 |

1. INTRODUCTION

1.1 INTENDED USE

3

The MICROSED-SYSTEM ESR analyzer is an automatic instrument for the analysis of the erythrocyte sedimentation rate. It constantly and simultaneously scans 10 test tubes which are custom-made for ESR analysis.

1.2 IMPROPER USE

Following uses are considered improper:

- 1) Use of the device to obtain results different from ESR
- 2) Use tubes different from those specified in this manual
- 3) Every attempt to open tubes analyzed by the device
- 4) Use the device to analyze samples different from those specified

The above mentioned uses and every attempt to use the MICROSED-SYSTEM ESR analyzer with a purpose different from the intended use, must be considered improper.

2. SAFETY PRECAUTIONS AND POTENTIAL HAZARDS

2.1 ELECTRICAL EQUIPMENT

As in all electrical equipment the power supply is a potential source of danger. For this reason, avoid handling parts directly hooked up to the supply without disconnecting them. Never carry out maintenance on the equipment when it is under electrical tension. Until the equipment remains closed as supplied, the operator is protected against electric shock. The parts to pay attention to are: the power supply and the printer.

2.2 MECHANICAL EQUIPMENT

Never attempt to open the instrument. It contains moving parts which may cause injury.

2.3 SAMPLES

All the biological fluids must be considered potentially infectious by operators. Even if for the execution of the analysis the blood is not handled (because the operator must not remove the tube stopper), the operator has to adopt the national and international standards of precautions to avoid the biological danger. The same rules must be adopted by the technical-qualified assistance operator when intervenes on this instrument.

2.3.1 NOTES ON SAFETY MEASURES

The operator must pay a special attention to the sample collection. Must use the correct vacuum test tubes described for this equipment in this manual, since these tubes have been studied to aspirate the right level of blood.

Every attempt to put the blood into test tubes different to the one described, brings serious dangers of infection due to the risk of sample coming out, and this, moreover, will damage the optical part inside the instrument and provoke the loss of the guarantee. Refer to the tubes instructions for use to have more detailed information. On the instrument, to assure a correct use of the instrument, may be placed the following symbols:



Caution



In vitro diagnostic medical device



Consult instructions for use

2.4 USER PRECAUTIONS

Before beginning work with the analyzer, the operator, to protect himself from any danger, must know the rules for handling potentially infectious materials and for the Electro-mechanical systems.

2.5 RESIDUAL RISKS

Despite of the measures taken in the designing of the machine to guarantee a safe use of it, there might happen reasonably predictable occurrences, whose risk was possible to reduce, but not to eliminate completely.

| RESIDUAL RISKS | PROTECTION MEASURES |
|--------------------------|---|
| Biological contamination | The operator must always wear gloves and protection glasses, as prescribed by laboratory regulations. Do not ever open tubes. |
| Tubes breaking | Insert and remove tubes from holes maintaining a vertical position, without applying lateral forces. |

3. DISPOSAL AND RECYCLING

Herewith we declare that this instrument is subject to the European Directive 2012/19/EU (WEEE Directive). Therefore the instrument must be disposed separately, not as urban waste and delivered to the specific collection center in according to the Directive 2012/19/EU. The user can ask to the dealer the collection of the instrument if a new instrument is ordered to replace the old one.

On the instrument there is a label with the symbol shown in this page. The symbol means that the instrument can not be disposed as urban waste.



4. INSTALLATION

4.1 SYSTEM DESCRIPTION

The MICROSED-SYSTEM ESR analyzer is an automatic instrument exclusively employed for analysis of the erythrocyte sedimentation rate. Its total absence of commands, its precision and its ability to obtain the result already corrected to a temperature of 18°C (according to Manley) in only 15 or 30 minutes, make the MICROSED-SYSTEM ESR the most innovative and versatile system for this kind of analysis. It constantly and simultaneously scans 10 test tubes which are custom-made for ESR with this system.

MICROSED-SYSTEM follows the sedimentation of each sample independently, memorizing levels for the whole period of analysis. This allows the instrument to be used for random loading of the samples and for a continuous loading up to a capacity of 10 test tubes at a time. When the first sample is analyzed, it can be replaced by another one, so it is possible to achieve up to 40 tests/h.

MICROSED-SYSTEM has been conceived to simplify ESR analysis as much as possible, avoiding sample manipulation and operator's infection risk. To perform the analysis, the operator must simply place the sample test tube directly into the instrument. The result appears on the display in only 15 or 30 minutes. When the compensation of the result is active, the MICROSED-SYSTEM surveys the room temperature and converts the result to the reference temperature of 18°C (Manley). This is necessary in order to avoid considerable variations of values due to different room temperatures.

4.1.1 POWER SUPPLY

The analyzer is provided with an external power supply with low voltage output. The power supply comes along with the analyzer.

4.1.2 DISPLAY

An LCD display with back-lighting, allows constant monitoring of the analyses and visualization of the results. Sample or system error messages may also be displayed.

4.1.3 READING PLATE

One row of 10 test tube positioning channels, numbered from 1 to 10.

4.1.4 BAR CODE READER (OPTIONAL)

An external barcode reader can be connected to the instrument with a special cable. The cable can be requested with the code: EEE30-099 – "Cable MSS10C04 printer, barcode". The barcode reader must be an RS232 port standard model, with its own power supply unit. The barcode scanner configuration must be set with the following serial port setting:

- 9600 bps, 8 data bits, no parity, 1 stop bit, no handshake control signals.

4.1.5 PRINTER (OPTIONAL)

A printer can be connected to the instrument, it prints out ESR results and sedimentation graphs, according to the loading sequence, whenever an analysis is completed. It is external so it can be easily replaced.



Printer Technical Data: Type DPT-100

| | |
|--------------------|---|
| Power supply input | Direct powered from MICROSED-SYSTEM serial RS 232 |
| printing type | thermal |
| columns | 24 |
| conformity | CE |

4.1.6 TEST TUBES

The unique test tubes that can be used with this instrument are MONOSED®; a Vacuum Tube expressly made to be used with the MICROSED-SYSTEM. They contain sodium citrate at 3,2% and have a fixed vacuum to draw blood:

- PRD-PRV11B-50
- PRD-PRV11V-50 (for high altitudes).



4.1.6.1 Tubes handling requirements

The vacuum test tube needs to be inserted properly into its holder to obtain the automatic draw of blood required for the analysis. Tubes are removed from the holder only after the draw has been terminated completely, i.e. the required amount of blood for the analysis has been properly evacuated.

If an incorrect blood collection occurs, MICROSED-SYSTEM will refuse to analyze the sample. It will indicate a “lev” (level) error, because the Sedimentation Rate would be incorrect due to an erroneous ratio with the anticoagulant present in the tube. All vacuum test tubes need to be mixed gently immediately after blood collection, to ensure a proper mixing of the sodium citrate with the freshly drawn blood.

Therefore, tubes are gently turned completely upside down five times, ensuring that the air-bubble floats correctly from one end of the tube to the other. ESR tests should be carried out no later than 4 hours after blood collection, if samples are kept at room temperature: Refer to Tubes instructions to perform this operation correctly.

4.1.6.2 Tubes storage requirements

Store the test tubes at room temperature, always below 25°C. Never place the bench top tube container near a heating device or a window where direct sunlight could create an unwanted heating effect.

4.2 RS232 CONNECTOR DESCRIPTION AND I/O DATA FORMAT

NOTE: Data format is: 9600 bps, 8 data bit, 1 stop bit, no parity, hardware protocol RTS-CTS for printer, no protocol for barcode scanner.

Instrument 9 pin female connector:

| PIN | DIRECTION | NAME | DESCRIPTION |
|-----|-----------|------|--|
| 1 | --- | --- | (Do not connect!) |
| 2 | INPUT | RXD | Barcode data input |
| 3 | OUTPUT | TXD | Printer / Host data output |
| 4 | OUTPUT | DTR | Data Terminal Ready |
| 5 | --- | GND | Ground |
| 6 | --- | --- | (Do not connect!) |
| 7 | OUTPUT | +12 | Power supply for external custom printer |
| 8 | INPUT | CTS | Clear to send |
| 9 | --- | --- | (Do not connect!) |

DIRECT HOST CONNECTION CABLE EXAMPLE

Note: The connectors of the cable are 9 pin.

| Male (instrument) | Female (to host) |
|-------------------|------------------|
| 2 ----- | 3 |
| 3 ----- | 2 |
| 4 ----- | 8 |
| 8 ----- | 4 |
| 5 ----- | 5 |

5. MICROSED-SYSTEM START UP

5.1 POSITIONING OF THE ANALYZER

The MICROSED-SYSTEM must not be placed near centrifuges, oscillating agitators or other vibrating instruments which might cause movement of the bench. Please, keep in mind that the ESR is very sensitive to vibrations that could cause a false increase of results. The bench must be flat and level. Direct light on the instrument and sudden changes of temperature should be avoided.

5.2 INSTRUMENT STARTUP

Check the instrument configuration for your needs, see paragraph 5.3 for switches information.

Connect power supply outlet to the instrument. Insert the power supply plug in a socket with an earth connection. If the instrument has an optional printer and/or a bar code scanner, they should be connected to the MICROSED-SYSTEM with the appropriate cable and plugged in. Connect and switch-on first the printer, then the MICROSED-SYSTEM using the switch situated at the rear side of the instrument. Each time it is switched on, MICROSED-SYSTEM carries out an electronic initialization and an instrument self test. The following messages will appear:

```
Self Test Start...
```

During the self test, the instrument checks electronics parts and which kind of configuration is set. The following messages will appear:

```
print curve ON...  
printer OK...
```

This message inform the user about the printer status and if the sedimentation is active or not.

```
check the printer!
```

If the printer is not connected to the device, this message will appear.

```
30/60' working time  
results: 30', 1h, 2h mm
```

This message informs the user on the reading time and on how results will be displayed and/or printed out.

```
18°C temp. of reference
27.5°C internal temp.
```

This message informs the user on the temperature correction status and on the temperature measured by the instrument. Once the Self test is finished, the following message will appear:

```
Self Test Ok...
```

Now the instrument is ready for the analysis. The result type and temperature are shown always in the display. In the bottom line of the display there are results values. The following screen is an example:


```
results: 1h                               temp.27.5°C
 5  6  7  7  8  9  10  11  12  13
```

5.3 DIP-SWITCH CONFIGURATION


- 1 - Enable results mm/30 minutes Westergren
- 2 - Working time selection (Off = 30' ; ON= 30/60'). Results 1/h or 1/h and 2/h Westergren
- 3 - Enable temperature compensation at 18°C (**switched ON as default**)
- 4 - Printer output enable (**note: turn off this switch if no printer is connected**)
- 5 - Enable sedimentation graphic printout
- 6 - Enable 15' of working time with results mm/h Westergren only
- 7 - Internal fan enable (**switched ON as default**)
- 8 - Enable DC power supply for external DPT100 thermal printer

NOTE: the function is active if the dip switch is on "ON" position.


DIP SWITCH CONFIGURATION EXAMPLES




dip switch on: 3,4,7,8
 configuration : working time 30'
 results= mm/1h Westergren
 temperature compensation ON
 printer enable ventilation ON
 power supply printer ON



dip switch on: 3,4,6,7,8
 configuration : working time 15'
 results= mm/1h Westergren
 temperature compensation ON
 printer enable ventilation ON
 power supply printer ON



dip switch on: 2,3,4,7,8
 configuration : working time
 30/60 results= mm/1h and 2/h
 temperature compensation ON
 printer enable ventilation ON
 power supply printer ON



dip switch on: 1,2,3,4,7,8
 configuration : working time
 30/60' results= mm1/2h; 1h; 2h
 temperature compensation ON
 printer enable ventilation ON
 power supply printer ON

6. METHODS

6.1 WESTERGREN METHOD

This is the standard method in accordance with the Clinical and Laboratory Standard Institute (CLSI). It consists of a support that keeps the Westergren tubes, containing not coagulable blood, perfectly vertical and hermetically sealed. Westergren tubes have a diameter of 2.5 mm and are graduated up to 200 mm.

As soon as the sample is taken the venous blood is mixed with a sodium citrate solution at 3.8% (0.13 M), in the ratio of respectively four to one (1.6 ml + 0.4 ml of sodium citrate). The blood thus prepared and well mixed is drawn into a Westergren tube up to the zero mark. The tube is inserted in the appropriate support and the erythrocyte level is read after 60 min.

6.1.1 NORMAL ESR VALUES ACCORDING TO WESTERGREN

| Normal ESR Values | | |
|-------------------|--------|--------|
| | male | female |
| After 1 hour mm | 0 - 15 | 0 - 20 |

Greer, John P., MD., et al. (2004). Wintrobe Clinical Hematology (11th ed. Vol. 2, pp. 2697). Philadelphia: Lippincott Williams & Wilkins.

6.2 VARIATION OF ESR

Net increase of ESR (100 mm or more per hour)

1. Multiple myeloma and Waldenstrom macroglobulinemia
2. Malignant lymphoma
3. Leukemia
4. Serious anemia
5. Carcinomas
6. Sarcomas
7. Serious bacterial infections
8. Collagenosis
9. Biliary or portal cirrhosis
10. Ulcerous colitis
11. Serious nephrosis
15. Broken ectopic pregnancy
16. Menstruation
17. Normal pregnancy after the third month
18. Oral contraceptives taken
19. Tuberculosis
20. Post commissurotomy syndrome
21. Dextran administered intravenously

Moderate increase of ESR

1. Acute and chronic contagious diseases
2. Acute localized infections
3. Reactivation of a chronic infection
4. Rheumatic illness
5. Rheumatoid arthritis
6. Myocardial infarction
7. Malignant tumour with necrosis
8. Hyperthyroidism
9. Hypothyroidism
10. Lead or arsenic poisoning
11. Nephrosis
12. Internal hemorrhage
13. Acute hepatitis
14. Ectopic pregnancy
14. unbroken after the third month

Normality of ESR (most cases)

1. First stage acute appendicitis
1. (in the first 24 hours)
2. Precocious integral ectopic pregnancy
3. Malarial paroxysm
4. Cirrhosis of the liver
5. Arthrosis
6. Mononucleosis
7. Acute allergies
8. Viruses without complications
9. Peptic ulcer
10. Typhoid fever
11. Undulant fever
12. Rheumatic carditis with
12. cardiac decompensation
13. Whooping cough

Variation of the ESR due to External agents (once blood is in the tube)

- a) dilution ratio,
- b) bubbles
- c) strongly hemolytic samples
- d) sudden agitation
- e) temperature
- f) time after sample collection
- g) direct sunlight
- h) foam
- i) lipemic samples

7. OPERATING PROCEDURE


7.1 SAMPLES

7.1.1 SAMPLE COLLECTION

Samples must be collected following the vacuum technique, using only the right tube previously defined. During sample collection, wait until the test tube vacuum has completed the drawing of the blood in order to be sure of having drawn the right volume. See the tube's instructions for a correct use.

7.1.2 SAMPLE MIXING

If it is not possible to analyze samples immediately after the collection, samples must be mixed delicately by overturning for at least five minutes. Use a rotating laboratory agitator or a dedicated mixing device. The recommended rpm value for the mixer is 15 - 20 rpm.

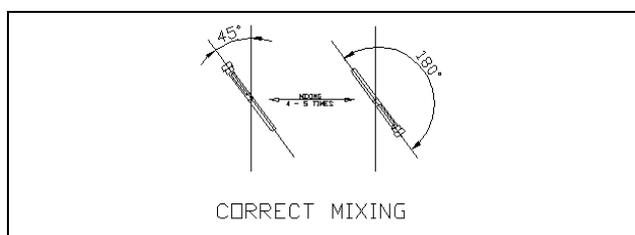

7.1.3 SAMPLE INSERTION

After mixing, the sample must be promptly transferred to the analyzer. It is also advisable to follow numerical sequence when loading channels. Every time a sample is inserted into a free channel an acoustic signal inform the user that the instrument recognized the tube. After loading the tenth, wait for the results and then remove analyzed samples from their channels before inserting new tubes. The sample positions on the plate are numbered from 1 to 10 but numbering is intended progressively in groups of 10. So when the tube in channel one is analyzed and removed, this position automatically becomes number 11 and so on.

7.1.4 SAMPLE IDENTIFICATION

If samples are identified by a barcode label, they can be identified using an external barcode scanner. The maximum ID length readable by the instrument is 12 digits. Do not overrun this limit. To perform this procedure correctly, follow these steps:

Read the barcode label

Insert the tube in the first free channel within 15 seconds form reading

The instrument will detect automatically the position of the new inserted tube and the ID will be automatically associated to that position. The display will show for some seconds:

```

+-----+
|New sample...          |
|Pos: 1  Pat.ID: 012345678912 |
+-----+
  
```

If a printer is connected, once the instrument finishes an analysis, the following information will be printed out:

Smpl.Chan.PatID# (no ID present)

1 1

30' 1h 2h

3 5 11 mm

Smpl.Chan.PatID# (ID: 123456789012)

1 1 123456789012

30' 1h 2h

3 5 11 mm

If the bar code is not available, to identify samples, write sample's ID on the label of each sample and prepare a report where to write the sample ID and the correspondent channel of the instrument where the sample has been inserted.

7.1.5 SAMPLE REMOVAL


As soon as sample has been analyzed, the result will be automatically printed out if a printer is connected. Results will stay on the display until the tube removal. Remove tubes carefully, maintaining tubes in vertical position, in order to avoid tubes breaking.

If the tube is removed before the end of the analysis, the instrument prints "rem" (removed) error.

7.2 TUBES LABELING

Identify the sample by writing on the original test tube label or by applying a bar code label. Follow the scheme to carry out this action correctly. In the figure the test tube "A" has the correct blood level and the original label on which to write the patient code or any other relevant data if the bar code label is absent. The part marked "H" shows the transparent zone that must be absolutely free and clear to allow the infrared rays to recognize the end of the blood column. The next test - tube "B" shows the correct position for the label. Test- tubes C and D illustrate how erroneous applications of the labels obstruct the reading of the analysis. If the MICROSED-SYSTEM Analyzer is installed in the surgery, the sample can be immediately analyzed by placing samples in a free position. Anyway the sample should be analyzed within three hours, paying attention to external agents shown below that might alter ESR in the pre-analysis phase.

3

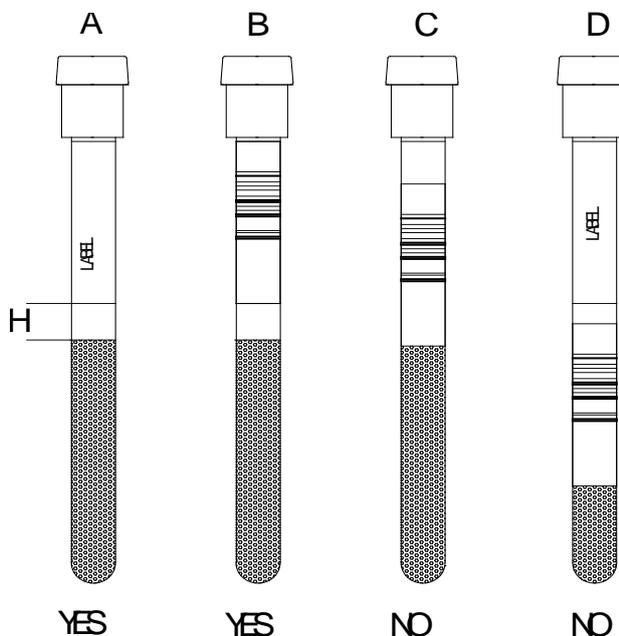

7.3 ANALYSIS

7.3.1 REMAINING TIME

During sample analyses, on the display appears for each sample the following symbol as indication of the remaining analysis time.



time remaining symbols

7.3.2 RESULTS PRE-INDICATION

Approximately 10 minutes after tubes insertion, the following symbols will appear on the display, giving a pre-indication of the results:

| % of Sedimentation at 10 minutes | | Symbol |
|----------------------------------|--|--------|
| < 16 | | -- |
| < 40 | | +- |
| >= 40 | | ++ |

This is only a pre-indication and it can't be used as final result.

Please note, pre-indication is shown only on 30 and 60 minutes reading mode.

7.4 CALIBRATION PROCEDURES

7.4.1 INSTRUMENT CALIBRATION

Each instrument is pre-calibrated by the manufacturer and it does not require a user re-calibration. The calibration of each instrument is traceable from the serial number of the instrument.

7.4.2 TEMPERATURE CORRECTION

The obtained results are correlated to the method of reference related to the room temperature. MICROSED-SYSTEM, constantly measuring the analysis temperature, further reconverts the values obtained to the reference one of 18 degrees using the Manley table thus ensuring better reproducibility instead of analyses performed at different temperatures.

Manley table

| Correct T | Analysis Temperatures | | | | |
|-----------|-----------------------|------|------|------|------|
| | 18°C | 15°C | 18°C | 20°C | 25°C |
| 5 | 4 | 5 | 5 | 6 | 8 |
| 10 | 9 | 10 | 10 | 12 | 16 |
| 20 | 18 | 20 | 21 | 25 | 31 |
| 30 | 27 | 30 | 31 | 37 | 45 |
| 40 | 36 | 40 | 42 | 49 | 58 |
| 50 | 46 | 50 | 52 | 60 | 71 |
| 60 | 55 | 60 | 62 | 71 | 82 |
| 70 | 63 | 70 | 72 | 82 | 93 |
| 80 | 72 | 80 | 82 | 93 | 104 |
| 90 | 81 | 90 | 93 | 103 | 114 |
| 100 | 90 | 100 | 103 | 114 | 125 |

MICROSED-SYSTEM converts the results to 18 degrees as per the table if analysis room temperature is between 15 and 32 degrees.

7.5 ERRORS AND WARNINGS

7.5.1 WARNINGS INFORMATION

These Messages may appear on the display :

LEV: Indicates that the sample level is not into the range permitted by the instrument.

REM: Indicates that the test tube has been removed from the position in which it had been placed.

The test tubes are checked in their positions every second. Do not touch the test tubes during the whole period of analysis because, for the reason described, the result will be lost.

7.5.2 SYSTEM ERROR WARNINGS

"MEC ERROR: system stopped..." or "ERROR: call service..."

These warnings will be given if the instrument should find problems with the mechanical movement of the reading plate. After this indication the instrument will definitely stop its operation and the technical service must be called.

7.5.3 SERVICE

In case of malfunctioning of the instrument, service can be made only by authorized personnel.

Only technicians with a certificate which states that they have followed a service training in ELITechGroup or made by a ELITechGroup authorized person, can operate service on the instruments.

If a technician is not available, defective instruments can be sent to ELITechGroup after calling the technical service.

Please contact your instrument distributor.

8. INTERNAL QUALITY CONTROL

Good Laboratory Practices suggest to test every day at least one control (1 normal and 1 abnormal) to check if the instrument is working correctly. ELITechGroup developed a special Sedimentation Control for ESR values. This control simulates the behavior of normal and abnormal human blood and can be used to test the instrument's performances. Controls must be tested exactly as normal patient's samples and results should be recorded on Quality Control Charts. Each laboratory can establish its own acceptability ranges. Refer to Sedimentation Control package insert for more detailed information.

9. PERFORMANCE CRITERIA AND LIMITATIONS

9.1 PERFORMANCE CRITERIA

| | |
|---|--|
| Mechanical/ Optical resolution of detection: | 0.2 mm |
| Automatic temperature conversion to 18°C. (Manley table): | Accepted range: Range 15° - 32°C. |
| Level range for correct analysis: | From 50 to 60 mm from the bottom of the Monosed ESR tube |
| 2 measuring points: | Initial and Final |
| Measuring range: | 1 - 140 mm/h |
| Results pre-indication: | After about 10 minutes |
| Precision, within run: | CV ≤ 10% (for samples with an ESR > 30 mm/h) |
| Correlation: | |
| | <i>R value</i> <i>n</i> <i>Regression line</i> |
| 30 minutes working time | 0.98 55 $y = 1.0129x - 0.7772$ |
| 15 minutes working time | 0.97 55 $y = 1.1309x - 3.3716$ |

9.2 LIMITATIONS

Strongly lipemic or hemolytic samples may alter reading capability.

Sed rate values > 140 mm/h will be indicated with this mark only.

10. MAINTENANCE

Due to component parts simplicity, MICROSED-SYSTEM does not require special maintenance. The most sensitive part is the infrared sensors inside the instrument.

Pay attention to the cleanliness of reading plate; when not used, it must be covered with the dust cover supplied along with the reader.

Do not clean the reading plate with liquids.

The entry of liquids or solid material into channels can cause considerable damage to the instrument.

10.1 CLEANING INSTRUCTIONS

Dust can be removed using an ordinary vacuum cleaner. It is advisable to clean once a month the instrument externally with a disinfectant solution to reduce the microbial contamination. Concerning test tubes, they must remain well closed and the cap should absolutely not be removed. The label must be correctly positioned and well stuck to the test tube surface. Label fragments could fall into the test tube and obstruct a correct reading function during analysis.

11. TROUBLESHOOTING GUIDE

Before calling for a service technician, please check the handling of sample collection, mixing procedures and operating instructions.

| ALARM OR TROUBLE | CAUSE | REMEDY |
|---|---|---|
| LEV | a) Sample level high or low b) The label was not placed in its proper position. | a) Repeat sample collection b) Replace label and repeat analysis |
| REM | Sample has been removed | Repeat analysis |
| T.ERR | “Temperature error” sensor malfunction | Data-analysis is not converted to 18°C. Call service assistance |
| MEC. ERROR or ERROR call service | Motor or mechanical malfunction | Call service assistance |
| Data result is not printed | a) Printer power b) Printer cable c) Instrument printer configuration | a) Check power supply b) Check cable c) Check instrument configuration d) Replace printer |
| Data result seems not correct | a) Sample clot b) Sample has foam c) Sample measured after 4 hours from sample collection d) Sample short mixing e) Temperature conversion is OFF | a) Repeat sample collection b) Remix gently c) Check instrument configuration |
| One or more samples are shown on the display without tubes introduced | a) Paper pieces or dust on sensors b) Internal cable problem | a) Call service assistance |
| Barcode reading not work | a) Adapter cable problem b) Scanner power problem c) Wrong ID procedure | a) Check adapter cable b) Check power of the scanner c) Read the user manual |
| No info on display | a) Instrument switch problem b) Instrument power problem c) Internal problem | a) Check instrument switch b) Check power supply unit c) Call service assistance |
| PRINTER NOT READY..... Message | a) Printer is not connected b) Printer out of paper c) Printer cable problem | a) Connect the printer or turn off printer configuration. b) Load a new roll of paper b) Check the printer cable |
| Analysis end delay on display | a) Printer is not connected but enabled b) Printer out of paper c) Printer cable problem d) Random samples inserted, the reading plate is moving | a) Connect the printer or turn off printer configuration. b) Load a new roll of paper c) Check the printer cable d) NO PROBLEM, results are always correct |
| Analysis end delay on printer | Random samples inserted, the reading plate is moving | NO PROBLEM, results are always correct |

12. TECHNICAL SPECIFICATIONS

| | |
|--|--|
| Area of application: | Blood sedimentation rate analysis |
| Instrument size: | Height 140 mm, Width 180 mm, Depth 100 mm |
| Weight: | About 0.9kg |
| Instrument input power: | 12 Vdc 1.5 A (external power supply unit) |
| External power supply unit input power: | 100 - 240 Vac 50/60 Hz |
| Operating Conditions: | Temperature 15°C – 32°C room temperature Humidity: 45% - 85% not condensed |
| 4 Reading channels: | 10 Nuskaitymo kanalai |
| 6 Reading time (selectable): | 15, 30 or 60 minutes Nuskaitymo laikas |
| Analytical capacity: | Max 40 tests/h |
| Loading pattern: | Random |
| Blood draw level acceptance from | 50 to 60 mm for Monosed ESR tubes |
| Measuring method: | IR beam |
| Reading resolution: | 0,2 mm |
| Results resolution: | 1 mm/h |
| Temperature correction: | Automatic compensation referred to 18°C (Manley) |
| Results (selectable): | 3 In Westergren mm/30', mm/1h, mm/2h. |
| Interface: | Single RS 232 port for printer output and barcode scanner input |

13. BIBLIOGRAPHY

- 1) THYGESEN, J.E.(1942). The mechanism of blood sedimentation. Acta Medica Scandinavia, Suppl. 134.
- 2) WINTROBE,M.M. and Landsberg, J.W. (1935). A standardised technique for the blood sedimentation test.
American Journal of Medical Sciences, 189, 102
- 3) HARDWICKE, J. and SQUIRE, J.R. (1965). The basis of the erythrocyte sedimentation rate. Clinical Science, 11, 333
- 4) International Committee for Standardisation in Haematology (1977). Recommendation for measurement of erythrocyte sedimentation rate of human blood. American Journal of Clinical Pathology, 68,505
- 5) LASCARI, A.D. (1972). The erythrocyte sedimentation rate. Paediatric Clinics of North America, 19,1113
- 6) MANLEY, R.W. (1957). The effect of room temperature on erythrocyte sedimentation rate and its corrections. Journal of Clinical Pathology, 10, 354