

35 pirkimo dalis



Kam rizikuoti dėl

kraujo infekcijų?

Įrodyta ir indikuota, kad „Tegaderm CHG“ tvarstis mažina su kateteriais susijusių kraujo infekcijų (CRBSI) bei kolonizacijos ties kateteriu riziką. Tokia indikacija yra tik skaidriam I. V. tvarščiai.

- Kliniškai įrodyta, kad centrinės venos ir (arba) arterijos kateterius turintiems pacientams, CRBSI rizika sumažėjo 60 proc.¹
- Kliniškai įrodyta, kad centrinės venos ir (arba) arterijos kateterius turintiems pacientams pagrindinės su kateteriais susijusios infekcijos rizika sumažėja 67 proc.¹
- Kliniškai įrodyta, kad centrinės venos ir (arba) arterijos kateterius turintiems pacientams, kolonizacijos ties oda ir kateteriu rizika sumažėja 61 proc.¹
- Iki septynių dienų užtikrina vienodą antimikrobinį poveikį.²
- Tvarstį „viskas viename“ lengva naudoti, kaip ir „3M™ Tegaderm™“ I. V. tvarstį.
- Skaidrus, todėl patogus stebėti kateterio įvedimo vietą.

„3M™ Tegaderm™ CHG“ chlorheksidino gliukonato I.V. tvarsčiai

Patikima apsauga, kuria



Su kateterio įvedimu susijusios kraujo infekcijos (CRBSI) yra vienos sunkiausių ir sudėtingiausių su sveikatos priežiūra susijusių infekcijų (HCAI), kurių gydymas brangiai kainuoja, dėl jų reikia ilgiau likti ligoninėje, gali prasidėti ligos ar net ištykti mirtis.

Pramonės, vyriausybės ir klinikų iniciatyvos stipriai sumažino CRBSI riziką, kaštus bei dažnumą, tačiau net ir vieno CRBSI atvejo yra per daug.

Net jei tokių infekcijų pasitaiko retai, CRBSI riziką galite dar labiau sumažinti, naudodami „Tegaderm CHG“ tvarsčius.

Įrodyta – sumažina su kateterių įvedimu susijusias rizikas


Didžiausiame kada nors atliktame atsitiktiniame kontroliuojamame tyrime (RCT), skirtame įvertinti CHG turinčius gelinius tvarsčius (4 163 kateterių buvo įvesta 1 879 pacientams), nustatyta, kad „Tegaderm CHG“ tvarsčiai gerokai sumažina CRBSI riziką, naudojant kartu su kitomis geriausios praktikos intervencijomis¹ (žr. 1 pav.).

- **Indikuota ir kliniškai įrodyta**, kad centrinėje venoje ar arterijoje kateterius turintiems pacientams, pagrindinės su kateteriais susijusios infekcijos (pagrindinės CRI) rizika sumažėja 67 proc.¹ (žr. 2 pav.).
- **Indikuota ir kliniškai įrodyta**, kad centrinės venos ir arterijos kateterius turintiems pacientams, sumažėjo kolonizacijos ties kateteriu rizika (žr. 3 pav.).
- Stebėjimo tyrimuose nustatyta, kad sumažėjo su centrine linija susijusių kraujo infekcijų (CLABSI) atvejų.³
- Įrodyta, kad po odos paruošimo⁴, tvarsčiai **iki septynių dienų nuslopina odos floros dauginimąsi** ir efektyviai kovoja su įvairiais klinikinio požiūriu svarbiais mikroorganizmais⁵, įskaitant atsparias atmainas².
- Nuo mikrobu septintą dieną saugo taip pat efektyviai, kaip ir pirmą dieną².
- Sugeria skysčius (prakaitą, kraują ir išskyras) nepakenkiant antimikrobinėms savybėms⁶.
- Įrodytas CHG gelio **antimikrobinis poveikis** sunkiomis eksperimentinėmis sąlygomis, naudojant kateterį ir kraujo baltymus. Tyrimo rezultatai rodo, kad dėl gelio poveikio, CHG kateterį buvo galima įvesti po kateteriu².


1 pav. Su kateteriu susijusios kraujo infekcijos



2 pav. Pagrindinės su kateteriu susijusios infekcijos

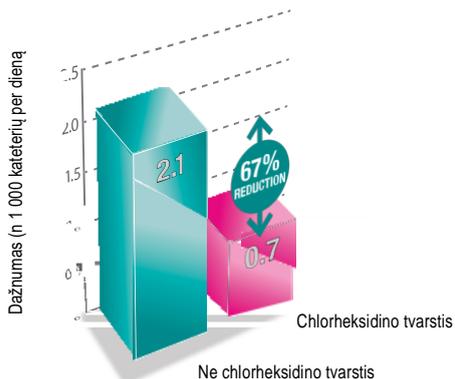

3 pav. Kolonizacija ties kateteriu

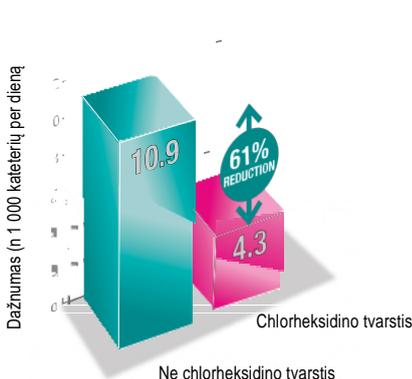

galite pasikliauti

„Viskas viename“ antimikrobinis skaidrus tvarstis – patogus ir saugus


- „3M™ Tegaderm™“ plėvelė suteikia galimybę nuolat stebėti įvedimo vietą.
- „Tegaderm“ plėvelė su 2 proc. chlorheksidino gliukonato gelio pagalvėle atitinka kūno formas ir prisitaiko prie paciento judesių.
- Pusiau peršlampama ir visiškai orui laidi plėvelė leidžia pasišalinti drėgmei.
- CHG nereikia papildomos drėgmės ir jis nuolat veikia, kad apsaugotų.

Išskirtinė apsauga

- Sutvirtinti kraštai ir saugumą garantuojantys grioveliai.
- Minkšti prilimpantys kraštai aplink kateterio įvedimo vietą suformuoja apsauginę zoną.

Suderinama su I. V. vietos geriausiomis priežiūros praktikomis ir protokolais

- Sukuria hermetišką, sterilų barjerą nuo išorinių teršalų, įskaitant skysčius, bakterijas ir virusus*.
- Kaip ir rekomenduoja CDC 1A gairės bei infuzijos praktikos standartai, leidžia nuolat stebėti įvedimo vietą ir matyti, ar neprasidėjo infekcija.^{7,8}
- Pagal INS ir CDC apibrėžimą, tvarstis laikomas kateterio tvirtinimo priemone ar stabilizavimo įtaisu.^{7,8}
- Atlikus atsitiktinį kontroliuojamą „Tegaderm CHG“ tvarsčio tyrimą nustatyta, kad jis atitinka „Epic³“ rekomendaciją dėl chlorheksidinu impregnuotų tvarsčių naudojimo su centrinės venos kateteriais.⁹

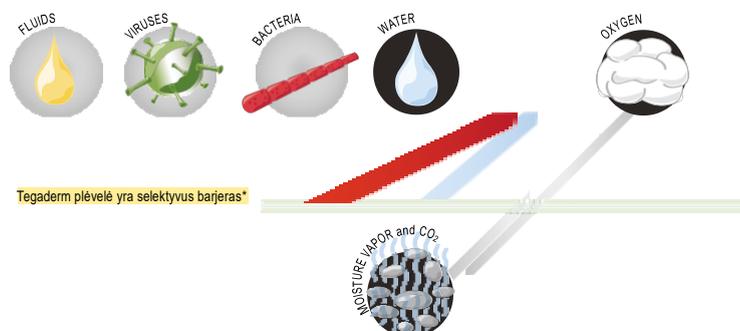

Tvarstis yra pralaidus orui ir leidžia pasišalinti drėgmei bei tuo pat metu apsaugo nuo teršalų, įskaitant tuos, kurie dažniausiai sukelia su kateteriu susijusias kraujo infekcijas.

Nepralaidus vandeniui, skysčiams virusams, bakterijoms, leidžiantis kvėpuoti odai tvarstis - plėvelė

**In vitro* tyrimai rodo, kad skaidri „Tegaderm CHG“ tvarsčio plėvelė sukuria 27 nm skersmens arba ilgesnį barjerą nuo virusų. Tvarstis tvirtai laikosi ir yra nepralaidus.¹⁰
Pastaba. „Tegaderm CHG“ tvarstis nėra skirtas pakeisti siūles, reikalingas naudojant trumpalaikius centrinės venos kateterius (pvz., jungo, poraktikaulinėje, šlaunies venose).

Literatūra

1. Timsit JF, et al. Randomized Controlled Trial of Chlorhexidine Dressing and Highly Adhesive Dressing for Preventing Catheter-Related Infections in critically ill adults. *American Journal of Respiratory and Critical Care Medicine* 2012; 186 (12):1272-1278.
2. Karpanen TJ, et al. (2011) Antimicrobial activity of a Chlorhexidine intravascular catheter site gel dressing. *Journal of Antimicrobial Chemotherapy*, 66: 1777-1784.
3. Scheithauer S, Lewalter K, Schröder J, Koch A, Häfner H, Krizanovic V, Nowicki K, Hilgers RD, Lemmen SW. Reduction of central venous line-associated bloodstream infection rates by using a chlorhexidine-containing dressing.
4. Bashir MH, et al. (2012) Suppression of regrowth of normal skin flora under chlorhexidine gluconate dressings applied to chlorhexidinegluconate-prepped skin. *American Journal of Infection Control*, 40(4):344-8.
5. Hensler J, et al. (2009). Growth inhibition of microorganisms involved in catheter-related infections by an antimicrobial transparent IV dressing containing Chlorhexidine gluconate (CHG). ECCMID, Helsinki, May 2009.
6. Schwab D (2007). Absorption of saline, human blood and plasma by Tegaderm CHG gel pad and BIOPATCH dressing. 3M data on file, Study-05-010658.
7. Centers for Disease Control and Prevention. Guidelines for the Prevention of Intravascular Catheter-related Infections.
8. Infusion Nursing Standards of Practice Supplement to Jan/ Feb 2006 Vol 29, 1S ISSN 1533-1458.
9. H.P. Loveday, et al. epic3: National Evidence-Based Guidelines for Preventing Healthcare-Associated Infections in NHS Hospitals in England. *Journal of Hospital Infection* 86S1 (2014) S1–S70.
10. Arrowsmith, M (2012) Bacterial & Viral Barrier Claim For 3M Tegaderm CHG I.V. Securement Dressings. 3M Data on file.

„3M™ Tegaderm™ CHG“ chlorheksidino gliukonato I.V. tvarsčiai

„Tegaderm CHG“ dar geriau apsaugo I. V. vietą, nes naudojamas CHG. Prie didesnio saugumo taip pat prisideda skaidrumas, patikimumas ir „3M™ Tegaderm™“ tvarsčio naudojimo paprastumas.

Visiškai orui laidi skaidri plėvelė

- Nuolatinis įvedimo vietos stebėjimas.
- Atitinka kūno formas ir prisitaiko pacientui judant.
- Skatina drėgmės pasišalinimą ir patikimą prilaikymą.
- Sukuria hermetišką, sterilų barjerą nuo išorinių teršalų, įskaitant skysčius, bakterijas ir virusus*
- Be latekso
- Pusiau peršlampus ir orui laidus, kad geriau pasišalintų skysčiai bei pagerėtų prisitvirtinimas.

Sterilios juostelės

- Sukurta patikimam kateterio prilaikymui įvedimo vietoje.
- Atspausdintos etiketės tvarsčių keitimo dokumentavimui. Geresnis protokolo laikymasis.

CHG gelio pagalvėlė

- 2% chlorheksidino gliukonatas
- Sugerianti CHG gelio pagalvėlė saugo, esant kraujui, fiziologiniam tirpalui ir išskyroms.
- CHG išskiriamas iškart ir nuolat, todėl nereikia papildomai drėkinti.
- Lipnios CHG gelio pagalvėlės prisitaiko prie kateterio.

Geresnis kateterio prilaikymas

- Sutvirtinti krašteliai ir grioveliai, kad tvirtiau laikytųsi.
- Minkšto audinio kraštis puikiai prikimba ir suformuoja apsauginę zoną aplink kateterį.
- Raštuota plėvelė tvirtai prikimba, reguliuoja drėgnumą ir švelniai nusiima.
- Plėvelę prispaudus, klajai patenka į odos nelygumus ir padidina prikibimo plotą.
- Klajai sukietėja per 24 valandas.

Patogi naudojimo sistema su rankenėlėmis

- 2 rankenėlės, kad būtų patogiau uždėti neliečiant tvarsčio.
- Dėl konstrukcijos, uždedama tiksliai ir lengvai.
- Sumažina prikibimo prie pirštinių ar odos riziką.

Tvarstis su rėmeliu

*In vitro tyrimai rodo, kad skaidri „Tegaderm CHG“ tvarsčio plėvelė sukuria 27 nm skersmens arba ilgesnį barjerą nuo virusų. Tvarstis tvirtai laikosi ir yra nepralaidus.¹⁰

Užsakymo informacija

	GAMINIO KODAS	BENDRAS TVARSČIO DYDIS	GELIO PAGALVĖLĖS DYDIS	PASKIRTIS	NHSSC KODAI	TVARSČIŲ / DĖŽUČIŲ DEŽUTĖJE	DĖŽUČIŲ PAKUOTĖJE
3M p.d.	 1657R	8,5 cm x 11,5 cm	3 cm x 4 cm	Visi CVS, arterijų, dializės, vidurio linijos ir kiti perkutaniniai įtaisai	ELW294	25	4
	 1658R	10 cm x 12 cm	3 cm x 4 cm	Visi CVS, arterijų, dializės, vidurio linijos ir kiti perkutaniniai įtaisai	ELW625	25	4
	 1659R	10 cm x 15,5 cm	3 cm x 7 cm	PICC linijos, visi CVC ir kiti perkutaniniai įtaisai	ELW295	25	4
	 1660R	7 cm x 8,5 cm	2 cm x 2 cm	Visi CVC, vidurio linijos ir kiti perkutaniniai įtaisai	ELW366	25	4

Norėdami daugiau sužinoti apie „Tegaderm CHG“ tvarsčius arba visus „Tegaderm“ I. V. tvarsčius, apsilankykite adresu www.3m.com/tegadermchg

Daugiau informacijos suteiks vietinis „3M Critical and Chronic Care“ atstovas.

www.3m.co.uk/healthcare



3M Health Care Limited

3M House Morley Street
Loughborough
Leicestershire LE11 1EP
Tel.: (01509) 611611
Faks.: (01509) 237288

3M Ireland

The Iveagh Building
The Park
Carrickmines
Dublin 18, Ireland
Tel.: 00 353 (01) 280 3555
Faks.: 00 353 (01) 280 3509



„3M“ ir „Tegaderm“ yra „3M“ prekių ženklai.
© 3M 2014.
ANTT yra „Association for Safe Aseptic Practice“ prekės ženklas.

Aplankykite mus „Facebook“.



[facebook/3mtegadermivsolutions](https://www.facebook.com/3mtegadermivsolutions)

Nuskaitykite šį QR kodą.



GF308A

Product Description

3M™ Tegaderm™ and Tegaderm™ HP Transparent Film Dressings consist of a thin film backing with a hypoallergenic, latex-free adhesive that gently, yet securely, adheres to skin. Tegaderm™ dressings are breathable, sterile, transparent and waterproof, and provide a barrier to external contaminants.

Tegaderm™ HP Film has a special adhesive for greater holding power in the presence of moisture.

Specially designed Tegaderm™ dressings, with unique shapes and securing tapes provide solutions for difficult to dress wounds and I.V. catheters.

Product Features and Benefits

Versatile—one product to satisfy many clinical situations

Tegaderm™ dressings can be used to protect I.V. sites, enhance wound healing, prevent skin breakdown, and protect clean, closed surgical incisions.

Tegaderm™ dressings are available in many sizes, shapes and application styles to meet a wide variety of needs.

The frame allows the dressings to be tailored for special applications, when desired. Application systems of most other transparent dressings do not allow for this customization.

Easy to apply—unique frame delivery system

Application of Tegaderm™ dressing is intuitive and quick, making it easy to remember and easy to teach. It is especially convenient for patient self-care.

Tegaderm™ dressing minimizes application time and saves dressing waste and costs. The frame delivery system provides maximum control of the thin film for rapid application of even the largest dressings. The unique “picture-frame” allows precise and secure placement of the dressing every time. If the adhesive surface accidentally touches itself, the dressing can be separated and applied, eliminating wasted dressings.

Tegaderm™ dressing is also available in a first-aid style delivery system for the health care professional who prefers this application method.

Gentle adhesive—just the right balance in adhesive strength

Tegaderm™ dressings are made with a hypoallergenic, latex-free adhesive that is gentle to the skin, yet securely holds catheters and other devices in place.

Tegaderm™ dressing provides good initial adhesion without building to excessive levels over time. Even for dressings left in place for extended periods, the risk of patient discomfort and skin trauma is minimal when the dressing is properly removed.

The hydrophilic nature of the Tegaderm™ HP Film adhesive makes it exceptionally adherent and useful for moist conditions and difficult-to-dress areas. It provides extra holding power, reducing unscheduled dressing changes.

Breathable—lets oxygen in and moisture vapor out

The breathability of Tegaderm™ dressings allows moisture vapor and gas exchange, which is essential to maintain normal skin function under the dressing.

Patients can wear Tegaderm™ dressings for extended periods of time, with minimal risk of skin irritation or maceration, and without excessive proliferation of skin flora.


Waterproof, sterile barrier—impervious to liquids, bacteria and viruses*

Tegaderm™ dressing acts as a barrier to protect the I.V. site or wound from external contaminants such as bacteria, viruses,* blood and body fluids.

Because Tegaderm™ dressings are waterproof, patients may bathe, shower or swim, if the dressing is completely sealed around the catheter or wound.

Tegaderm™ dressing is sterile and remains so as long as the outer package is intact. Do not resterilize by gamma, steam, or E-beam.

Hipoderminiai klijai. Pleistras be latekso.

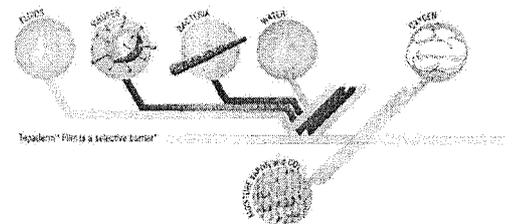

Tegaderm™ dressings are breathable, sterile, transparent and waterproof, and provide a barrier to external contaminants.

* *In vitro* testing shows that the transparent film of 3M™ Tegaderm™ brand dressings provide a viral barrier for viruses 27 nm in diameter or larger while the dressing remains intact without leakage.

3M™ Tegaderm™ CHG I. V. tvarstis (1657R)

Chlorheksidino gliukonato I. V. tvarstis

Naudojimo nurodymai



1

Atidarykite pakuočę ir išimkite sterilų „Tegaderm CHG“ tvarstį. Nuo lipnaus paviršiaus nuimkite apsauginę plėvelę. Tvarstį pasukite taip, kad lipnus jo paviršius būtų atsuktas į odą.



2

CHG gelinę pagalvėlę išcentruokite virš kateterio įvedimo vietos ir priglaudę palyginkite tvarščio kraštą. Prisiuvamų kateterių atveju, gelio pagalvėlę galima dėti tiek ant įvedimo vietos, tiek ant siūlių. Įtaisą reikia stabilizuoti pagal įstaigos protokolą.




3

Priglaudę palyginkite kitą skaidraus tvarščio kraštą.




4

Iš lėto nuimkite popieriaus rėmelį, tuo metu lygindami tvarstį, jį tvirtai spaudžiant, nuo centro link kraštų.

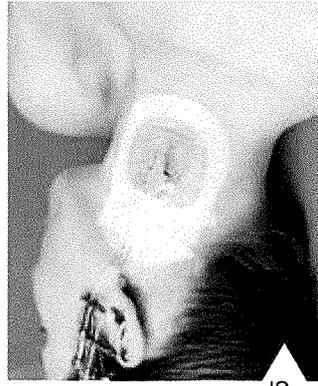

5

Užklijuokite juosteles, kad pritvirtintumėte kateterį. Vieną klijuokite po vamzdeliu, o kitą – ant vamzdelio.

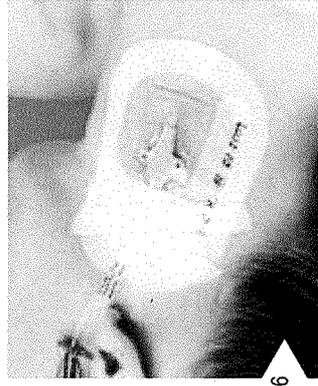

6


Duomenis apie tvarščio keitimą įtraukite į dokumentaciją pagal įstaigos protokolą. Užklijuokite dokumentuotą juostelę. Įrašykite kateterio spindį ar paiginimus.

Nuėmimo nurodymai

Tvarstį nuimkite pagal įstaigos protokolą arba jei jis persisunkęs. Kad patikrintumėte saturaciją, švelniai pirštu paspauskite gelio pagalvėlę. Jei spaudimo žymė nuo pagalvėlės neišnyksta, vadinasi tvarstį reikia keisti.

Nuimkite vamzdeliams tvirtinti naudotas juosteles.

Švelniai suimkite tvarščio kraštą ir iš lėto nuimkite tvarstį nuo odos. Judėkite link įvedimo vietos arba plaukų augimo kryptimi. Nuimkite iš lėto. Tvarščio staigiai neplėškite, nes galite pažeisti odą.

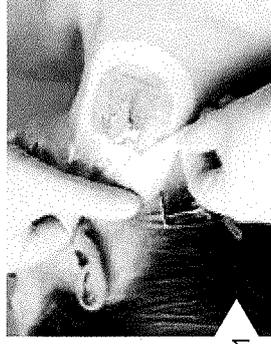

1



2



3

Tvarstį nuėmę, uždėkite nykštį ar smilų ant gelio pagalvėlės, kad pagreittumėte nuėmimą. „Tegaderm CHG“ tvarstį reikia nuimti nepažeidžiant gelio pagalvėlės. Tvarstį nuimkite judėdami link kateterio įvedimo vietos, priliaikydami odą ir kateterį, kad pastarasis neišitrauktų. Kad būtų lengviau nuimti, galima naudoti medicininę klijų šalinimo priemonę, tačiau jos prireikia ne visada.

3M Health Care

3M House Morley Street
Loughborough
Leicestershire LE11 1EP
Tel.: (01509) 611611
Faks.: (01509) 613326

3M Ireland Limited

The Iveagh Building
The Park
Carrickmines
Dublin 18, Ireland
Tel.: 00 353 (01) 280 3555
Faks.: 00 353 (01) 280 3509

www.3mhealthcare.co.uk

3M ir „Tegaderm“ yra 3M įmonės prekių ženklai.
© 3M Health Care Limited 2009.



Declaration of Conformity

As Legal Manufacturer
We, 3M Company, 3M Health Care,
3M Center, 2510 Conway Ave, Bldg. 275-5W-06
Saint Paul, MN 55144 USA

hereby declare under our sole responsibility
that the CE marked products to which this declaration relates,

3M™ Tegaderm™ CHG Dressing, Chlorhexidine Gluconate I.V. Securement Dressing,
Product Numbers:
1657R, 1658R, 1659R, 1660R, 1877R, 1879R

are classified,

per Rule 13 of Annex IX of the Medical Device Directive 93/42/EEC, as amended per 2007/47/EC
as a Class III device

and

are in accordance with Annex II of Directive 93/42/EEC, as amended per 2007/47/EC,
on the approximation of the laws of the European Member States concerning medical devices.

In addition, we declare that the above mentioned device fulfils the applicable provisions of the Directive 93/42/EEC,
as amended per 2007/47/EC.

and

are in conformity with the type described in the EC Design-Examination Certificate reference number: CE 525600
and the full quality assurance certificate CE 02242
delivered by British Standards Institute (BSI), Notified Body Number 2797

EU Representative Address
3M Deutschland GmbH
Health Care Business
Carl-Schurz-Str. 1
41453 Neuss, Germany

Signature: _____

Date: 16 December 2019

3M Health Care
Division Regulatory Affairs Manager
Medical Solutions Division

3M Tegaderm CHG I.V. Securement Dressing Receives FDA 510(k) Clearance for Expanded Indication to Reduce Catheter-Related Bloodstream Infection

ST. PAUL, MINN. June 6, 2017 – Catheter-related bloodstream infections (CRBSI) are life-threatening for patients and costly for the medical professionals and facilities caring for them. 3M is pleased to announce that the U.S. Food and Drug Administration (FDA) has recognized the efficacy of 3M™ Tegaderm™ CHG Chlorhexidine Gluconate I.V. Securement Dressing in reducing CRBSI, expanding the product’s 510(k) indication to include CRBSI reduction.

The expanded indication is supported by a randomized, multi-arm, controlled clinical trial of 1,879 subjects that found Tegaderm CHG I.V. Securement Dressing reduced CRBSI by 60 percent in patients with central and arterial lines ($p=0.020$).¹

“While we are making great strides in reducing CRBSI nationwide, these preventable infections are still responsible for significant morbidity, mortality and excess costs,” stated Pat Parks, MD, PhD, medical director for 3M Critical and Chronic Care Solutions Division. “Successful CRBSI prevention practices rely on dedicated clinicians using proven technology, such as Tegaderm CHG I.V. Securement Dressing, in alignment with current best practice standards.”

Tegaderm CHG I.V. Securement Dressing is the only transparent dressing indicated and proven to reduce CRBSI and vascular catheter colonization that aligns with evidence-based guidelines and practice standards. The dressing provides four essential elements to cover and protect patients’ catheter sites and secure devices to skin.

- Infection Reduction: Clinically proven to reduce CRBSI by 60 percent in patients with central and arterial lines. The dressing features an integrated gel pad containing 2 percent w/w CHG, a

¹ Timsit JF et al. *Randomized controlled trial of chlorhexidine dressing and highly adhesive dressing for preventing catheter-related infections in critically ill adults*. Am J Crit Care Med. 2012;186(12): 1272-1278
<http://www.atsjournals.org/doi/pdf/10.1164/rccm.201206-1038OC>.

well-known antiseptic agent with broad spectrum antimicrobial and antifungal activity that maintains antimicrobial activity for 10 days. Antimikrobinis poveikis išlieka 10 parų

- Site Visibility: Transparent film and gel pad allow for continual site observation, enabling early identification of complications at the insertion site.
- Consistent Application: Integrated CHG gel pad and dressing design ensure standardized, correct application.
- Catheter Securement: Designed to minimize catheter movement and dislodgement.

“Providing effective, proven technology such as Tegaderm CHG I.V. Securement Dressing is just one of the ways that 3M partners with clinicians to help them achieve their infection prevention goals,” said Parks. “We also provide clinical expertise and tools to support training and compliance, and engaging educational resources to help facilities implement the latest evidence-based guidelines and standards.”

For more information about coordinating a Tegaderm CHG Dressing product trial, please visit 3M.com/TegadermCHG.

###

3M and Tegaderm are trademarks of 3M Company.

About 3M

At 3M, we apply science in collaborative ways to improve lives daily. With \$30 billion in sales, our 90,000 employees connect with customers all around the world. Learn more about 3M’s creative solutions to the world’s problems at www.3M.com or on Twitter @3M or @3MNewsroom.

Contacts:

Jackie Vos, Inprela Communications
(612) 677-2022
Jackie@inprela.com

Nan Farnsworth, 3M
(651) 733-5747
nfarnsworth@mmm.com

LOT 33K8YC

REF 1657R

2024-04-16



(01)00707387782177
(17)240416(10)33K8YC

3M

Tegaderm™ CHG

- ⓐ Chlorhexidine gluconate I.V. Securement Dressing (Gel pad contains 2% w/w CHG)
- ⓑ Parsement au gluconate de chlorhexidine pour le maintien des cathéters intravasculaires
- ⓒ Chlorhexidin-Gluconat I.V.-Fixierverband
- ⓓ Medicazione di fissaggio I.V. con Clorexidina Glucosata
- ⓔ Adesivo con gluconato de clorexidina para fijación de catéters
- ⓕ Chlorhexidengluconat I.V. Verband
- ⓖ I.V.-förband med Korhexidin-glukonat
- ⓗ Forbinding med Korhexidin Glukonat til fastgørelse af I.V. katetre
- ⓘ Korhexidindglukonat I.V.-beskyttelsesbandasje
- ⓙ Koorteksidiniidglukonaatti I.V. -suojasidos
- ⓚ Penso I.V. som gluconato de Clorexidina
- ⓛ Повязка для фиксации внутривенных катетеров с хлоргексидина глюконатом
- ⓜ Хлоргексидин глюконатын Т етгін катетерді бекітуге арналган жапырма
- ⓝ テガダーム™ CHG クロキシジンゲル
- ⓞ 抗菌靜脈注射固定用防水透氣敷料
- ⓟ CHG 글루콘산 글로록세시딘 I.V. 고정 드레싱



STERILE EO
3 1/2 in X 4 1/2 in
8.5 cm X 11.5 cm
REF 1657R



CE 2797
Made in U.S.A. with globally sourced materials by 3M Health Care

2910 Sawyer Ave.
St. Paul, MN 55144, U.S.A.
(U.S.A.) 1-800-228-3957
3M.com/Tegaderm


3M Canada Company
P.O. Box 67, Box 9737
London, Ontario, N6A 4T1
1-800-364-5377
3M.com/Tegaderm

3M et Tegaderm are trademarks of 3M, used under license in Canada, unless sous licence au Canada.
© 2015, 3M. All rights reserved.

3M Deutschland GmbH
Health Care Business
Carl-Schurz-Str. 1
41453 Neuss, Germany

- Do Not Reseal
- Not Made with Natural Rubber Latex
- Do Not Reuse
- Do not use if package is damaged or open
- Caution, see instructions for use

Permatoma plėvelė per pusę kombinuota su neaustinio pluošto pleistru
Tvarsčio centre integruota antimikrobinio poveikio gelio pagalvėlė.
Gelio pagalvėlė ir tvarstis permatomi, todėl leidžia stebėti dūrio vietą.

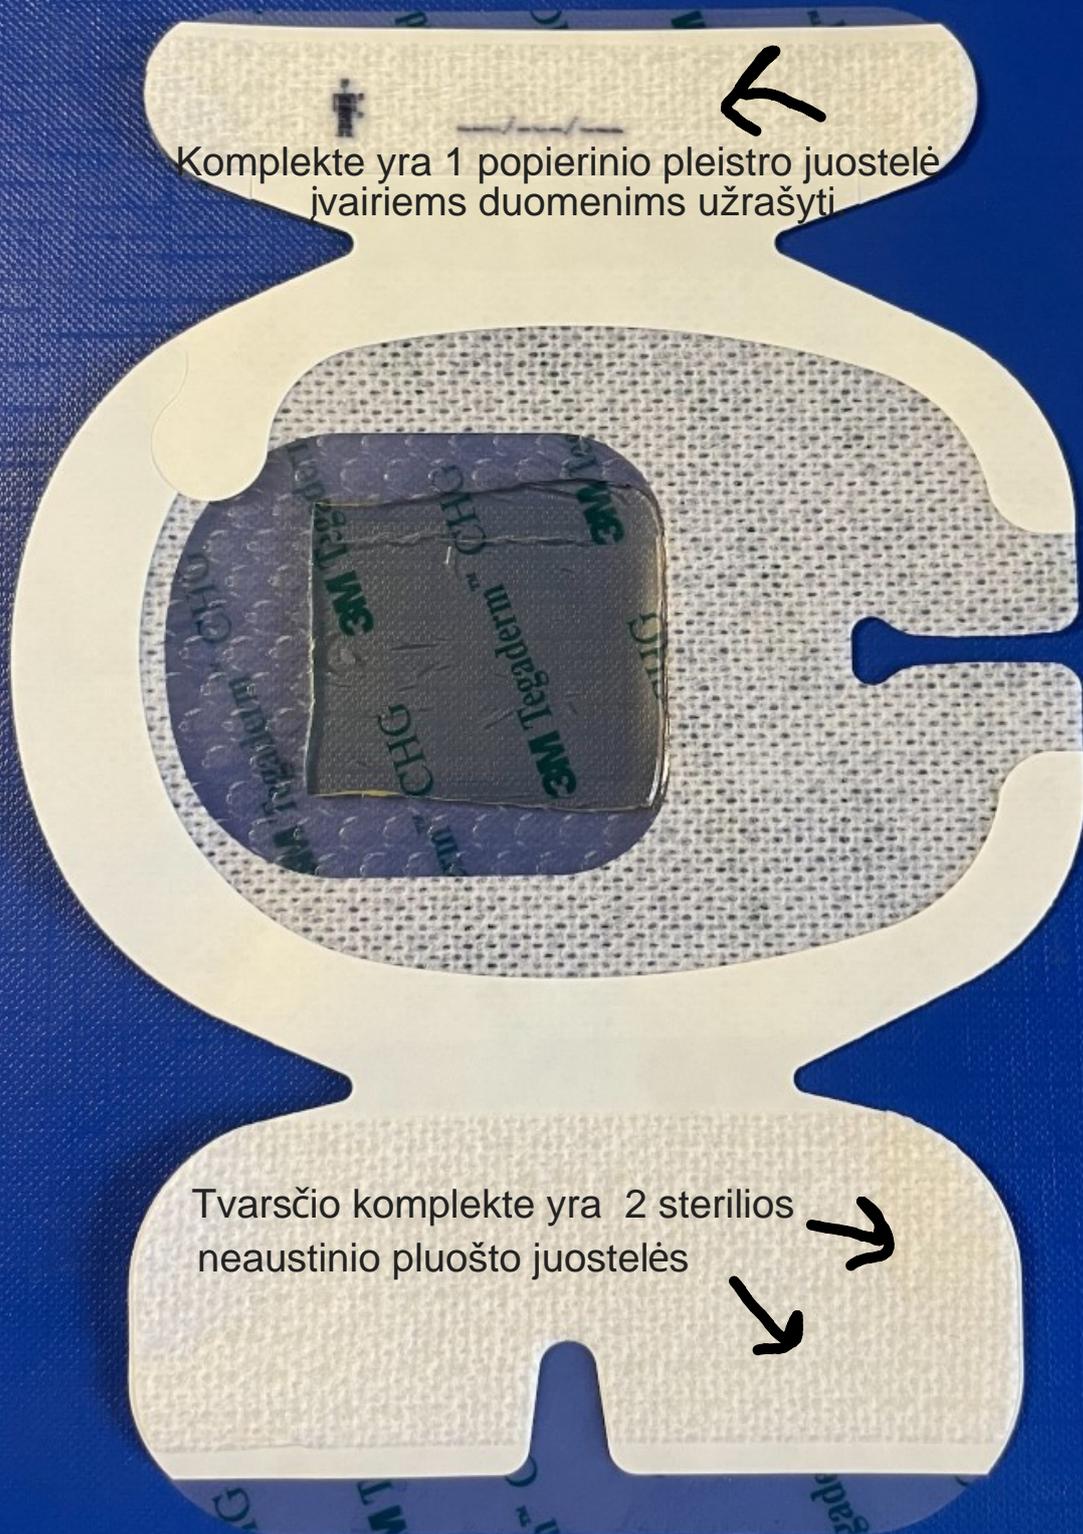



Tvarsčiai supakuoti steriliuose dalinai permatomuose įpakavimuose, kurie leidžia vizualiai, neatidarius įpakavimo, įvertinti tvarsčio dydžio tinkamumą.