



## Blood collection chair FK-02






**(2.5.)** Chair table 25x35 cm; load 15kg

Universal chair FK-02 is intended for injection procedures. The frame of the medical treatment chair is made of metal constructions, painted with powdered polymer paint and has four height-adjustable legs. **(2.2.)** The backrest is adjusted by means of a gas spring **(2.1)**. Two, all-adjustable armrests make the injection procedure easier on both the left and right sides of the patient. The chair has adjustment mechanisms for all major parts. All parts of the chair are made of non-allergenic, non-allergenic materials, easy to clean and disinfect, fire and swelling resistant. **(2.4.)** The legs of the chair are covered with clear plastic, which is resistant to abrasion and disinfectants. **(2.3.)**

Parameters	Model FK02
Backrest adjustment angle <b>(2.8.)</b>	0° - 95°
Total length of the shaft <b>(2.6.)</b>	170 cm
Width of the seat <b>(2.6.)</b>	50 cm
Overall width of the chair <b>(2.6.)</b>	71 cm
Trendelenburg position <b>(2.9.)</b>	from 0° to -3°
Adjusting the handles by means of a ball bearing <b>(2.7.)</b>	from -15° to + 65°
Permissible load <b>(2.10.)</b>	150 kg

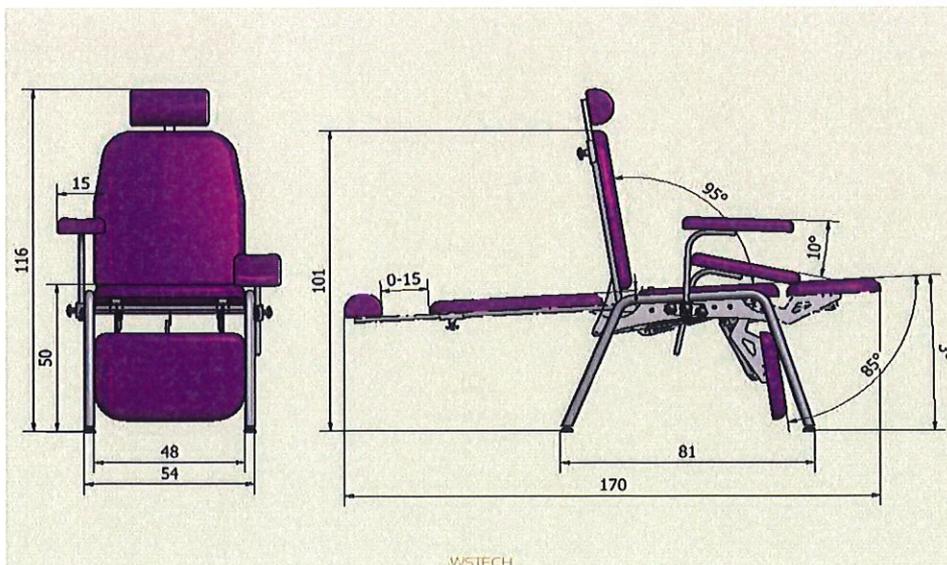

A