



VIVINEX IMPRESSED™ BE IMPRESSED



Set a new benchmark for visual
outcomes achieved by your
monofocal patients

Vivinex Impress™ enhances the intermediate vision of monofocal patients

Vivinex Impress™ IOL

RANGE OF VISION




NEAR


INTERMEDIATE



FAR

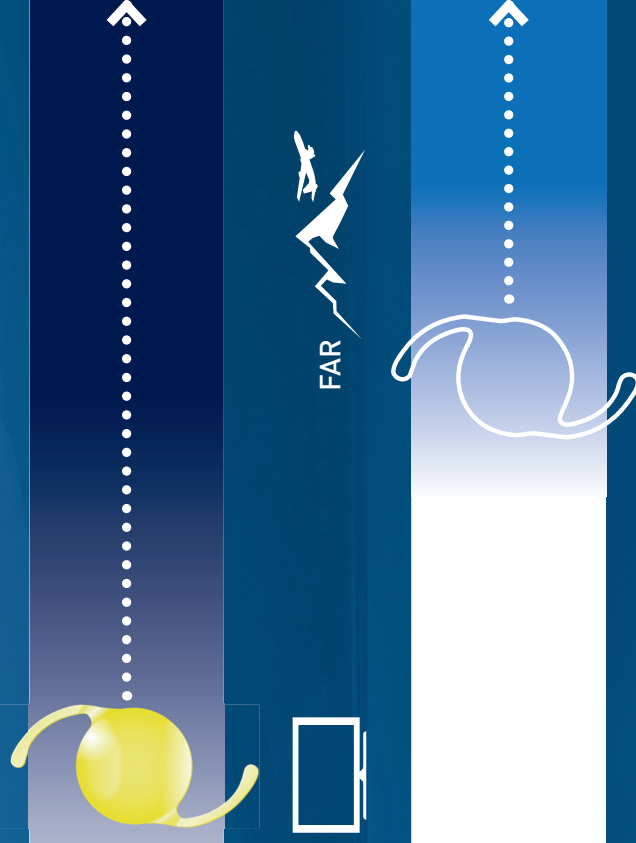


Standard monofocal aspheric IOL

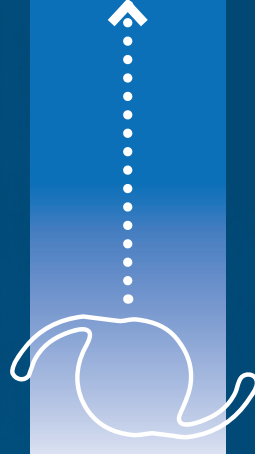


Vivinex Impress™ provides greater than 1 line of binocular visual acuity improvement at 66 cm

Interim results of a running multicentre study¹

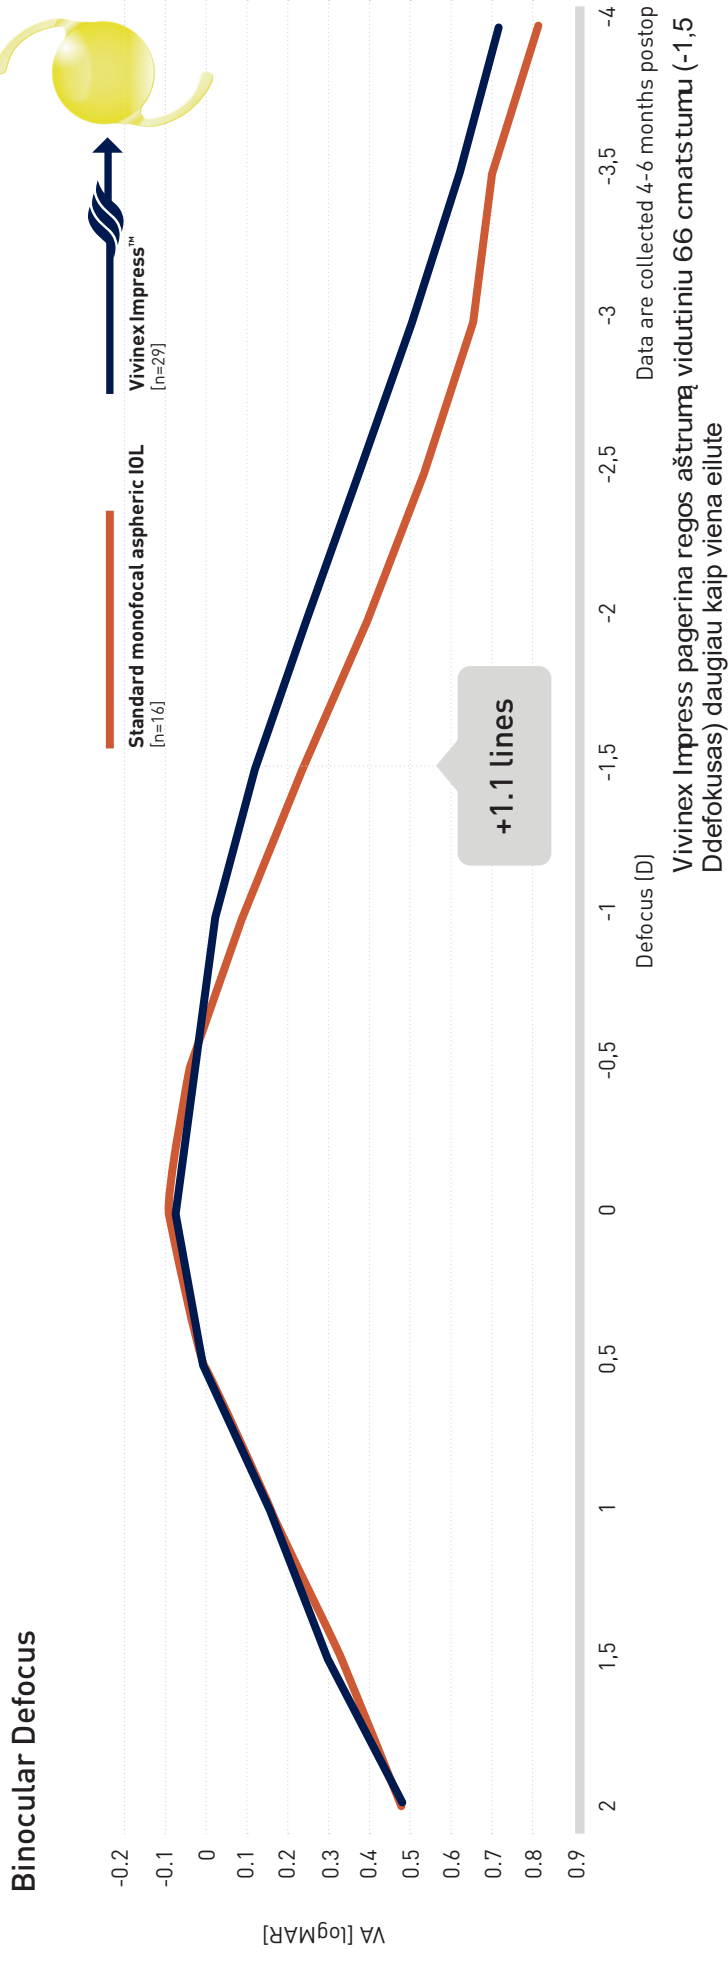


Vivinex Impress™ improves intermediate vision and provides consistent refractive predictability

Monocular distance-corrected visual acuity at 1 month¹

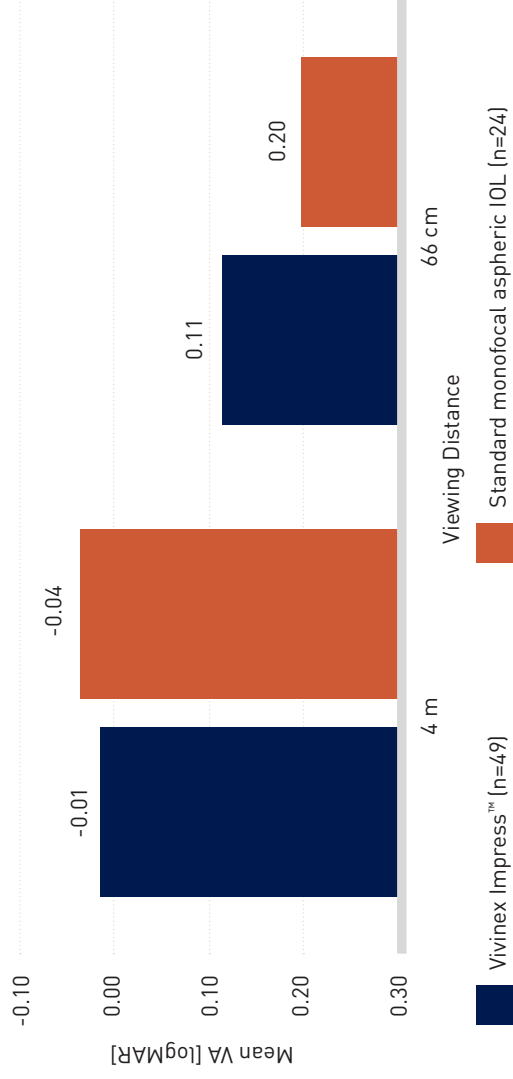

- No difference in best-corrected mean distance visual acuity at 4 m between Vivinex Impress™ and a standard monofocal aspheric IOL¹
- Approximately 1 line improvement in distance-corrected visual acuity at 66 cm in the Vivinex Impress™ group¹


Absolute value deviation from target postop spherical equivalent at 1 month¹

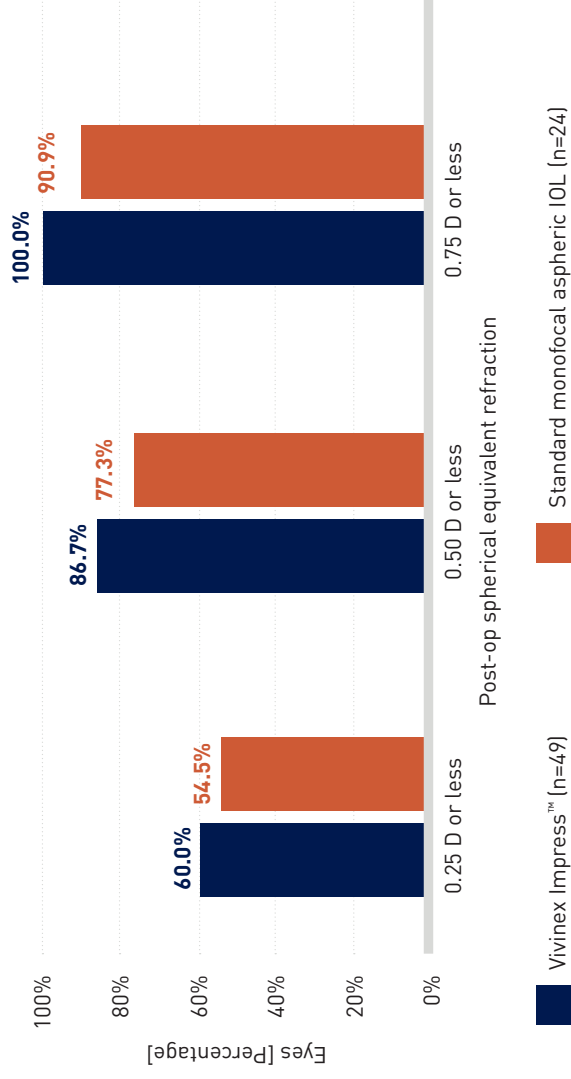

- Refractive predictability was excellent in both Vivinex Impress™ and the standard monofocal aspheric groups¹
 - within 0.25 D of target: 60% vs 55 %
 - within 0.50 D of target: 87% vs 77 %
 - within 0.75 D of target: 100% vs 91 %

So how does Vivinex Impress™ work?

Topographic representation of the Vivinex Impress™ anterior surface illustrates power variations

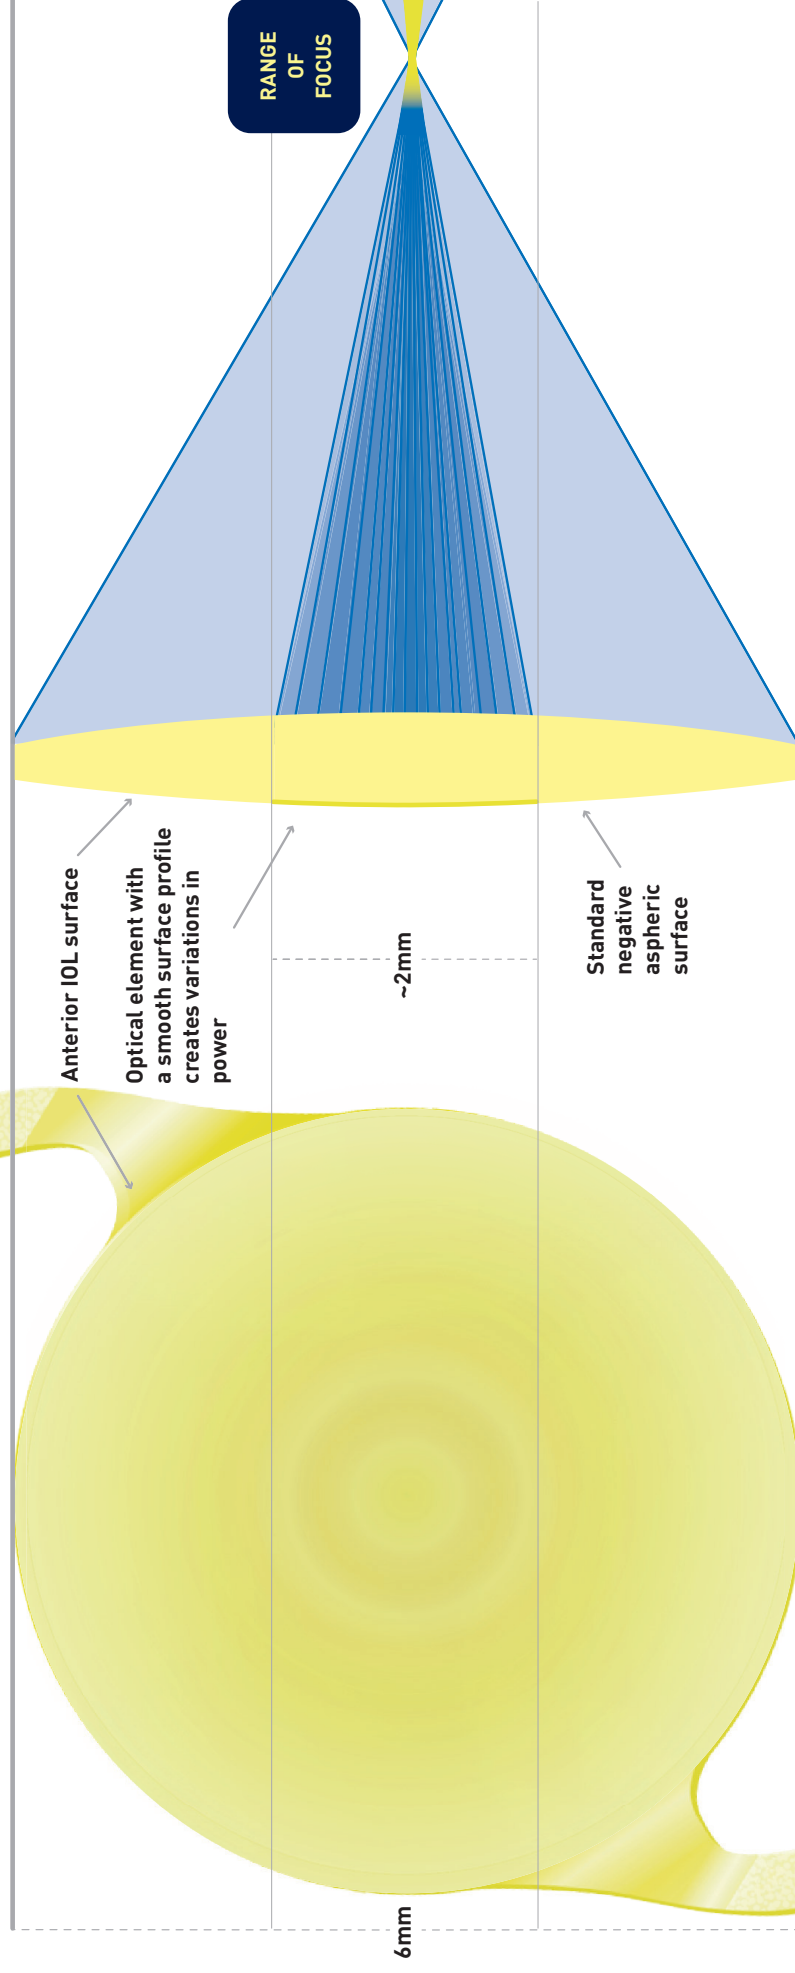

4

Centrinė optinė dalis modifikuotos laužiamosios galios, kas užtikrina pagilintą fokuso židinį ir pagerina regą vidutiniu atstumu.

The central optical element creates variations in power that provide an extended range of focus and improved intermediate vision. Vivinex Impress™ looks the same as a standard monofocal IOL.²

Benefits of the Vivinex™ platform



Glistening-free

Glistening-free hydrophobic acrylic IOL material^{3,4}



Improved Image Quality

Incorporates the Vivinex™ proprietary aspheric optic design which partially compensates for corneal spherical aberration and is more tolerant to sources of coma than standard aspheric designs⁵




Reduction of PCO

Active oxygen processing treatment, a smooth surface and square optic edge to reduce PCO^{3,6,7,8,9,10,11,12}



Smooth IOL unfolding and capsular bag stability


Textured rough haptic surface designed to reduce potential for adhesion to the optic surface during delivery, and provides better grip inside the capsular bag

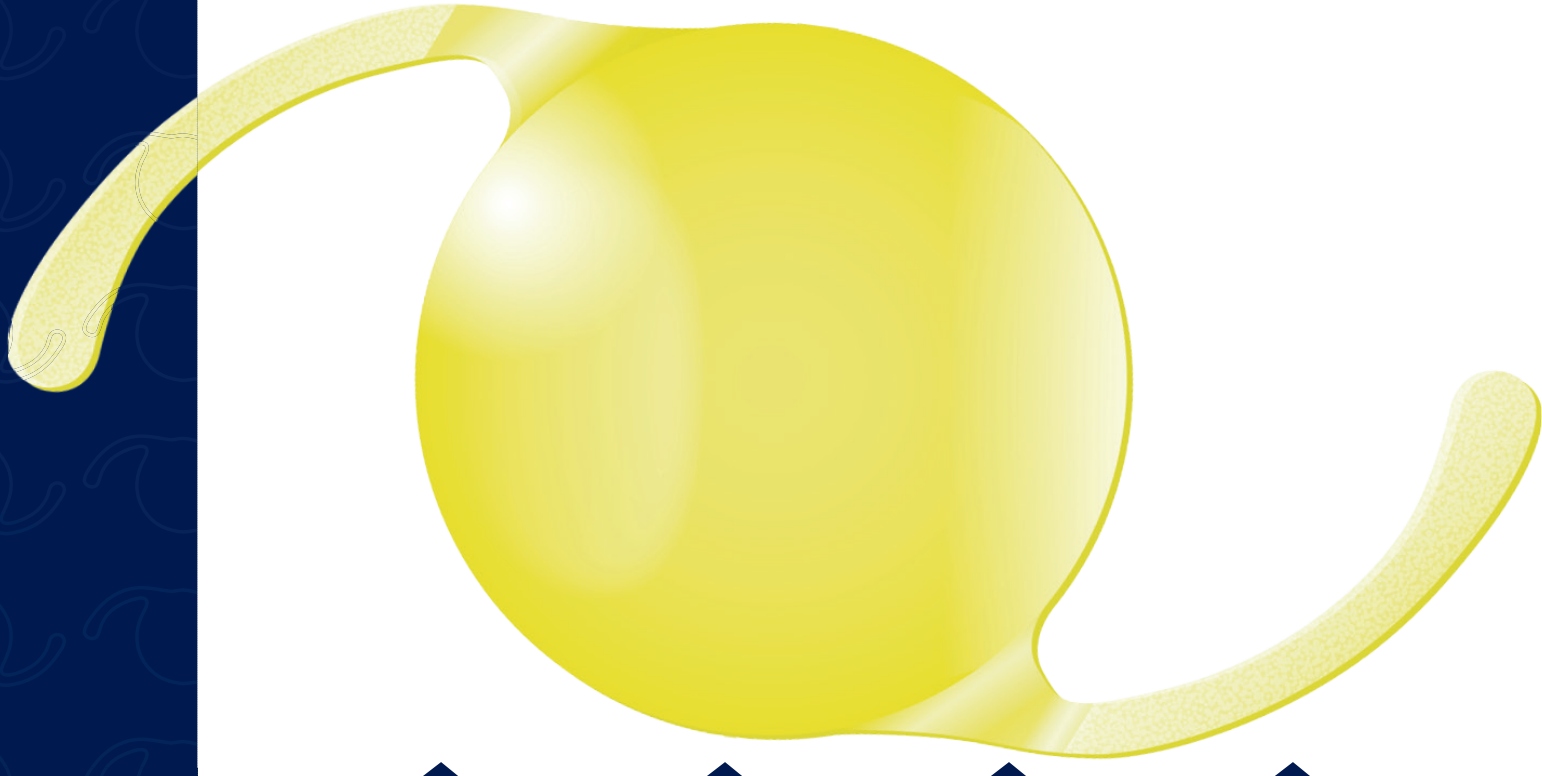


Delivered in the preloaded multiSert™ injector

Galimybė implantuoti stumiant arba sukanč rankenėlę ir galimybė kontroliuoti įvedimo gylį.


Push and screw modes and the ability to control insertion depth
Vivinex™ multiSert™ is a 4-in-1 delivery system that allows you to achieve outstanding delivery consistency with your choice of injection and insertion style¹³

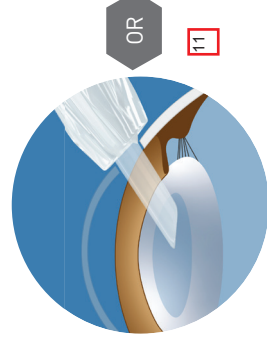

Delivery into capsular bag
insert shield:
Default position
Įvedimas į kapsulės maišą.
Įvedimo apsauga. Neaktyvuota



Delivery through incision wound tunnel
insert shield:
Advanced position
Įvedimas žaizdos kanale.
Įvedimo gylis apsauga aktyvuota.



Preloaded injectors are:

Easier to prepare, increasing safety by:^{14,15,16,17,18,19}

- Reducing risk of contamination and infection
- Reducing risk of IOL damage

More efficient in the OR:^{16,18}


- Minimising time spent preparing the IOL delivery system
- Creating fewer instruments to reprocess

More predictable:¹⁸

- Increasing predictability and consistency of IOL delivery

Specifications

Vivinex Impress™	
Model name	XY1-EM
Optic design	Abipus išgaubta optika su stačiu/aštriu, plonu pašiurkštintu kraštu Biconvex with square, thin and textured optic edge Anterior: Aspheric design Asferinis optikos dizainas
Optic & haptic materials	Hydrophobic acrylic Vivinex™ with UV- and blue light filter Hidrofobinis akrilinis su UV ir mėlynos šviesos filtru
Haptic design	Textured-rough haptic surface Atramiųjų elementų paviršius pašiurkštintas
Diameter (optic/OAL)	6.00 mm / 13.00 mm
IOL Power (Spherical equivalent)	+6.00 D to +30.00 D in increments of 0.50 D
Nominal A-constant*	118.8
Injector	multisert™ preloaded
Front injector tip outer diameter	1.70 mm
Recommended incision size	2.20 mm

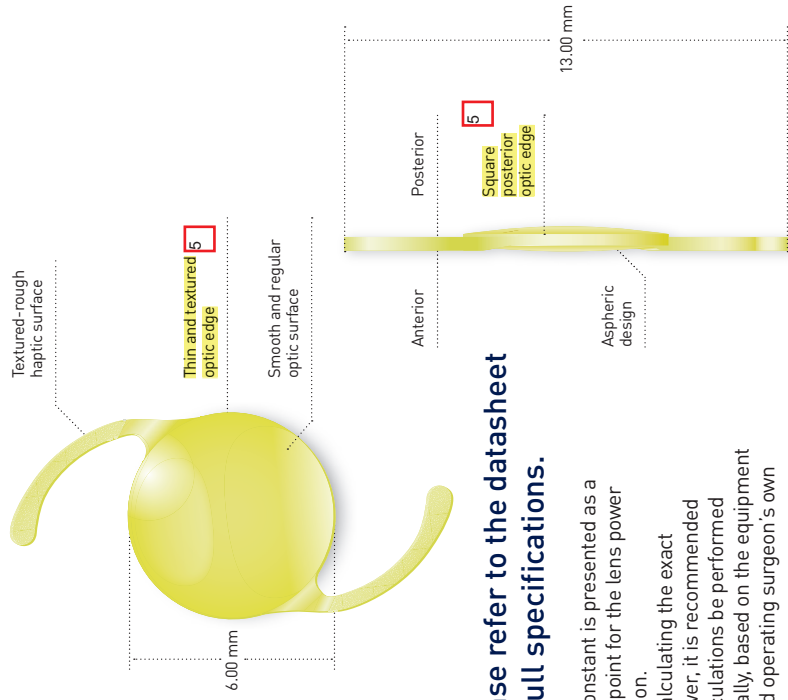

> Please refer to the datasheet for full specifications.

*The A-constant is presented as a starting point for the lens power calculation.
When calculating the exact lens power, it is recommended that calculations be performed individually, based on the equipment used and operating surgeon's own experience.



Delivered by the multisert™ preloaded injector



References: 1. HOYA data on file, CTM-23-P0105, HOYA Medical Singapore, Pte. Ltd. 2023 2. HOYA data on file RnD-20-367, HOYA Medical Singapore, Pte. Ltd. 2023 3. Tandogan, T. et al. [2021]. In-vitro glistening formation in six different foldable hydrophobic intraocular lenses. In BMC Ophthalmol 21, 126. 4. Auffarth et al. [2023] Randomized multicenter trial to assess posterior capsule opacification and glistenings in two hydrophobic acrylic intraocular lenses. 3-year results of a randomized trial. In: American journal of ophthalmology 217 [9], p. 224-231. 5. Giacinto, C. et al. [2019]. Surface properties of commercially available hydrophobic acrylic intraocular lenses: Comparative study. In: Journal of cataract and refractive surgery 45 [9], p. 1330-1334. 6. Werner, L. et al. [2019]. Evaluation of clarity characteristics in a new hydrophobic acrylic IOL in comparison to commercially available IOLs. In: Journal of cataract and refractive surgery 45 [10], p. 1450-1457. 7. Matsushima, H. et al. [2008]. Active oxygen processing for acrylic intraocular lenses to prevent posterior capsule opacification. In: Journal of cataract and refractive surgery 32 [6], p. 1035-1040. 8. Farukhi, A. et al. [2013]. Evaluation of uveal and capsule biocompatibility of a single-piece hydrophobic acrylic intraocular lens with ultraviolet-ozone treatment on the posterior surface. In: Journal of cataract and refractive surgery 39 [1], p. 113-122. 9. Nanavaty, M. et al. [2019]. Edge profile of commercially available square-edged intraocular lenses: Part 2. In: Journal of cataract and refractive surgery 45 [6], p. 847-853. 10. HOYA data on file, DoF-SERT-102-MULT-03052018, HOYA Medical Singapore Pte. Ltd. 2018 11. Edred, J. et al. [2019]. An In Vitro Human Lens Capsular Bag Model Adopting a Graded Culture Regime to Assess Putative Impact of IOLs on PCO Formation. In: Investigative ophthalmology & visual science 60 [1], p. 1081-1087. 12. Edred, J. et al. [2019]. Management strategies to reduce risk of postoperative infections. In Current ophthalmology reports, 11(4), 10.1007/s40135-013-0021-5. 13. Bodnar, Z. et al. [2012]. Toxic anterior segment syndrome: Update on the most common causes. In: Journal of cataract and refractive surgery, 38 [11], 1902-1910. 14. Jones, J. et al. [2016]. The impact of a preloaded intraocular lens delivery system on operating room efficiency in routine cataract surgery. In: Clinical ophthalmology (Auckland, N.Z.), 10, 1123-1129. 15. Park, C. et al. [2018]. Toxic anterior segment syndrome-an updated review. In: BMC ophthalmology, 18 [1], 276. 16. Chung, B. et al. [2018]. Preloaded and non-preloaded intraocular lens delivery system and characteristics: human and porcine eyes trial. In: International journal of ophthalmology, 11 [1], 6-11. 17. Schmidbauer, J. et al. Rates and causes of foldable and rigid intraocular lenses: clinicopathological analysis of 100 cases. In: Journal of cataract and refractive surgery, 28 [7], 1223-1228.

Information contained is intended for health care professionals. Please refer to the Instructions For Use for a full list of indications and contraindications. Some of the products and/or specific features as well as the procedures featured in this document may not be approved in your country and thus may not be available there. Design and specifications are subject to change without prior notice as a result of ongoing technical development. Please contact our regional representative regarding individual availability in your country. HOYA, Vivinex Impress, Vivinex and multisert are trademarks of the HOYA Corporation or its affiliates. ©2023 HOYA Medical Singapore Pte. Ltd. All rights reserved. HOYA Medical Singapore Pte. Ltd. | 455A Jalan Ahmad Ibrahim | Singapore 639939. Hoya Surgical Optics GmbH | De-Saint-Exupéry-Str. 10 | 60549 Frankfurt am Main | Germany | Hotline DE: Tel. +49 (0)800 664 2 664 | Fax +49 (0)800 774 2 774 hoya surgicaloptics.com

