


HOT SPAXUS™ Stent Delivery System

- Electrocautery-enabled delivery system

- kiekvienas stentas komplektuojamas su jo vienkartinę įdėjimo sistema su elektrokauterio galimybe;

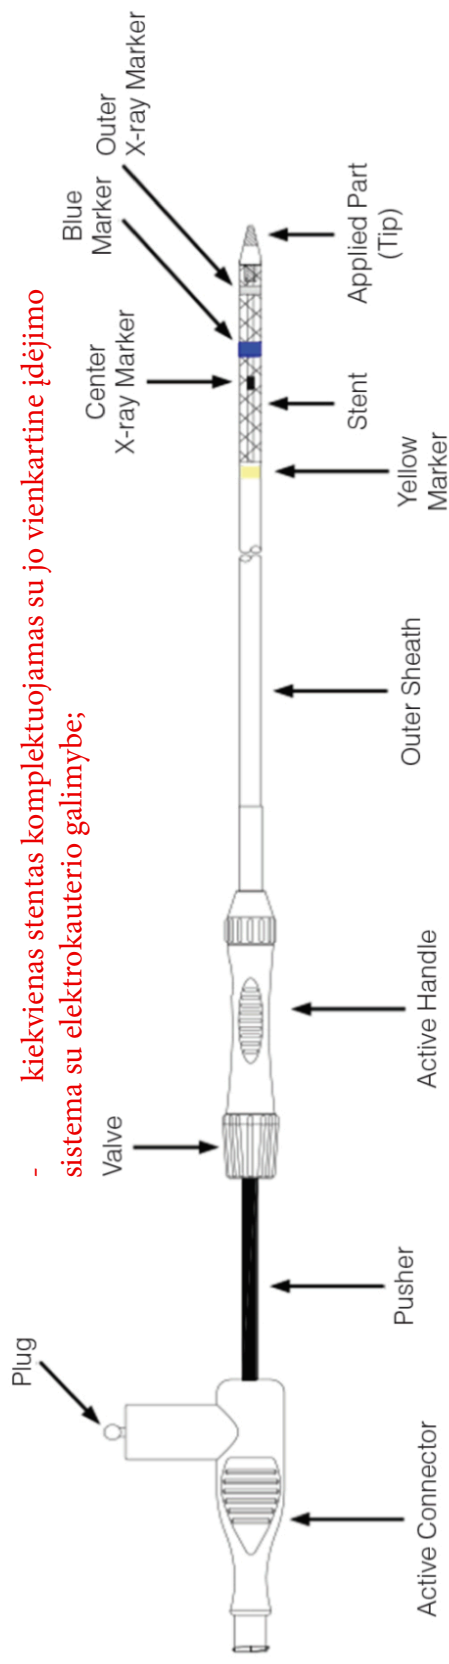

- When the outer X-Ray marker overlaps with the inner X-Ray marker:
→ The distal flange is completely opened.
- When the blue marker is visible under endoscopic view:
→ Start opening the proximal flange.

Blue marker on the outer sheath indicates accurate positioning during deployment of the proximal flange