



# magic


over 20 years of  
flow dependence

## ordering information

11 P.D

Reference	Total length (cm)	Guidewire max	Distal tip O.D.	Turquoise pursil O.D. (F) x L (cm)	White pursil O.D. (F) x L (cm)	Pink pursil O.D. (F) x L (cm)	Torver O.D. (F) x L (cm)
MAGIC1,2F	165	.008"	1.2F	1.2 x 12	1.8 x 3	2.4 x 30	2.7 x 114
MAGIC1,2FM	165		1.2F	1.2 x 3	1.8 x 12	2.4 x 30	
MAGIC1,2FM180	180		1.2F	1.2 x 3	1.8 x 17	2.4 x 40	
MA1,2FOLIVE	165		1.2F	1.2 x 12	1.8 x 3	2.4 x 30	
MAGIC1,5F	160	.009"	1.5F	/	1.5 x 15	2.4 x 25	2.7 x 114
MA1,5FMP	165		1.5F	/	1.5 x 20		
MA1,5FOLIVEMP	165		1.5F	/	1.5 x 20		
MAGICSTD	155	.010"	1.8F	/	1.8 x 10	2.4 x 25	2.7 x 114
MAGICMP	165		1.8F	/	1.8 x 20		

## magic compatibilities



Cyanoacrylate Glue\*



SPIF Flow Coil  
(e.g. pressure cooker)

\*MAGIC is glue compatible.

MAGIC, micro-catheters are intended for selective and hyperselctive vascular catheterization for diagnostic and therapeutic purposes. Class III CE0297 in compliance with Medical Device Regulation (MDR 2017/745). Manufactured by BALT EXTRUSION SAS. Carefully read the instructions for use before use. Not reimbursed. First CE marking:1998 The occlusion devices SPIF Flow Coil are intended for the embolization of vascular malformations of the vasculature. SPIF is class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT Extrusion SAS. Carefully read the instructions for use before use. First CE marking: 1998 (Magic); 2008 (SPIF). The content of this document, in particular data, information, trademarks and logos is BALT SAS's sole property. © 2022 BALT SAS and affiliates, all rights reserved. All representation and/or reproduction, whether in part or in full, is forbidden and would be considered a violation of BALT SAS and its affiliates' copyrights and other intellectual proprietary rights. This document with associated pictures is non-contractual and is solely dedicated to healthcare professionals and BALT's distributors (BALT's supplier's distributors). The products commercialized by BALT shall exclusively be used in accordance with the instructions for use included in the boxes. DC034GB (05/22)



Balt  
10, rue de la Croix Vigneron,  
95160 Montmorency, France  
Tél. : +33 (0)1 39 89 46 41  
Fax : +33 (0)1 34 17 03 46  
[www.baltgroup.com](http://www.baltgroup.com)



# magic


Flow dependent microcatheter

Intended for selective and hyperselective vascular catheterization for diagnostic or therapeutic purposes.

# unique alloy

pursil and torver

avm\* treatment

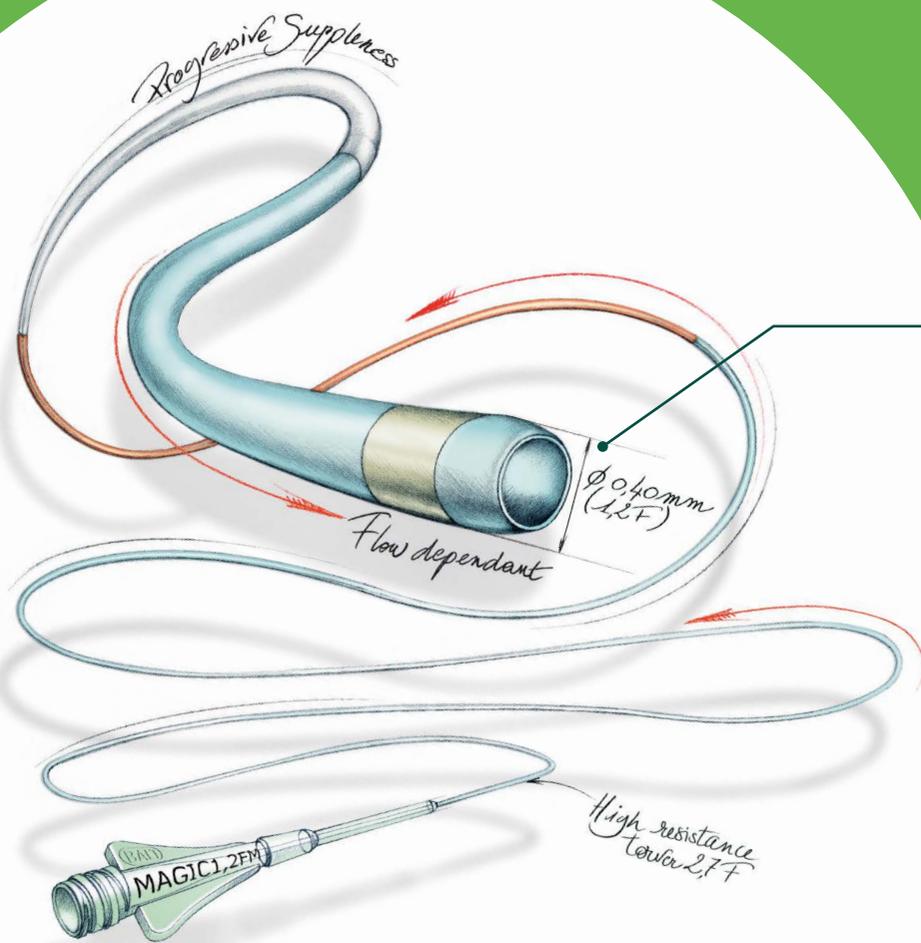

Flow dependent

MAGIC progression is facilitated by blood flow

Gentle navigation of the microcatheter inside distal and tortuous vasculature

● Distal access

The small size of the tip allows distal intracerebral hyperselective catheterism of small vessels

Unique alloy

In 1982, BALT developed an alloy that combines the mechanical resistance of polyurethane (PUR) and the flexibility of silicone (SIL): **PURSIL**

In 1987, another alloy called **TORVER** was introduced for the proximal part of the catheter



Up to **4** progressive suppleness transition zones

magic progression is facilitated by **blood flow**

\* Arteriovenous Malformation