

PHILIPS HEALTHCARE	<b>Product Recycling Passport</b>	Page 1 of 4
-----------------------	-----------------------------------	-------------

Product name	Expression Patient Monitor (Model MR400, REF 866185)
Identification code(s)	REF 866185
Total weight (in Kg)	44.75 kg (cart only); 50.2 kg (system)


Producer/ Manufacturer	Name company:	Philips Healthcare
	Address:	3000 Minuteman Rd. Andover, MA
	Zip code:	01810
	Country:	U.S.A


Recycle Info	Items:	Location
Special attention  	Plastics – PC + ABS Blend (total weight = 7.4 kg)	Cart, Lower processing unit, Modules
	Aluminum – Sheet Metal, Die Cast, Sand Cast (total weight = 7.07 kg)	Lower processing unit, Display, Patient Connections
	Zinc – Die Cast (total weight = 15.79 kg)	Base Casting
	Glass – Fiber Optic, Touch Screen (total weight = 0.82 kg)	Display, Cart
	Copper – Cables (total weight = 0.28 kg)	Lower processing unit, Display, Patient Connections
	Printed Circuit Boards (total weight = 1.12 kg)	Lower processing unit, Display, Patient Connections, Modules
	Packaging: - PE Foam – 3.65 kg - Wood – 12.98 kg - Cardboard – 6.04 kg	Packaging

  Fluids / Gases	Items:	Location
	N/A	

		Type:	Location
 <p>Batteries</p> <p>To be Removed</p>	989803169491 - (Panasonic) CGA103450A Lithium Ion (12 cell per pack; 4 packs per system) Weight per pack = 637.5 g		Cart lower processing unit
	989803191341 - (BAK) 383562PN Lithium Polymer Cell/Battery (1 cell per pack; 3 packs per system) Weight per pack = 30.2 g		Modules (2 packs for ECG, 1 pack for SpO2)
		Substances:	Location
<p>Hazardous</p>  <p>To be Removed</p>	PVC		Lower processing unit internal tubing
	PUR:		Sellable NIBP Trunk Hoses
	- 989803183221		
	- 989803183231		

Show locations of materials mentioned on the previous sheet.  
(Please use an illustration/drawing of the system, photos are discouraged)

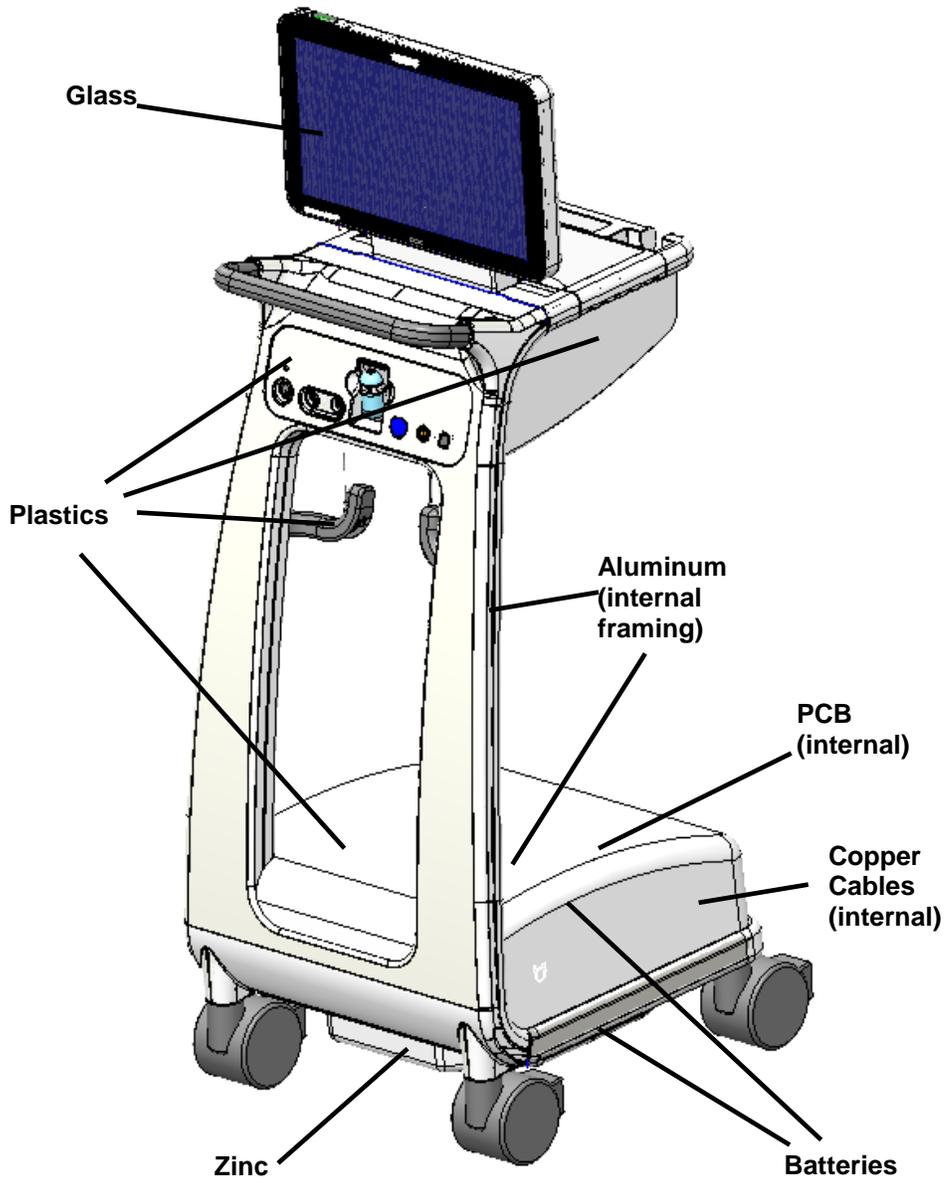

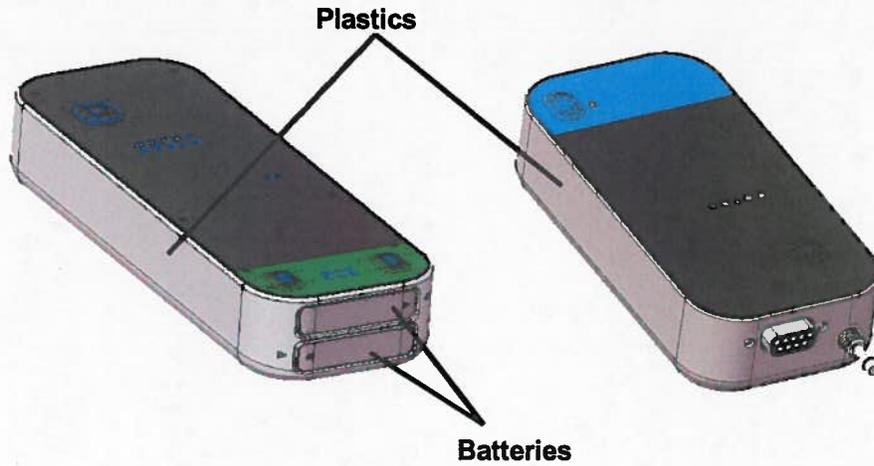


### Recycling Passport Revision History


Rev	Description	Date
A	As Issued	2015 May 07


### Recycling Passport Approval Signatures

(Note: Do not include the section below in the published version to protect privacy)

  
 Dimitri Kostakis 19-May-2015

 19-May-2015  
 Len Kovalsky

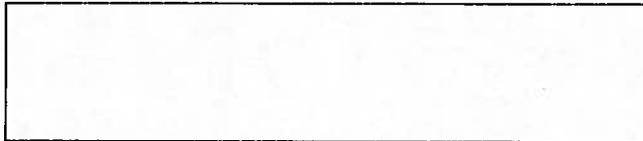

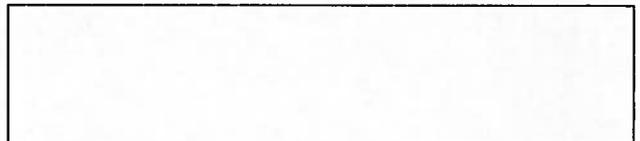

# Philips Healthcare

## Produkto perdirbimo pasas

Produkto pavadinimas: Expression Paciento monitorius (Model MR400, REF 866185)

Identifikacinis numeris: REF 866185

Svoris: 44.75 kg (tik dėžė); 50.2 kg (sistema)

Gamintojas: Philips Healthcare, 3000 Minuteman Rd. Andover, MA, 01810, JAV

Antrinio panaudojimo informacija:

Reikalaujamas ypatingas atidumas

Dalys	Lokacija
Plastikas – PC + ABS mišinys (bendras svoris = 7,4 kg)	vežimėlis, apatinis apdorojimo blokas, moduliai
Aliuminis – lakštinis metalas, lidinys, smėlio lydinys (bendras svoris = 7,07 kg)	Apatinis apdorojimo blokas, ekranas, paciento jungtys
Cinkas – lydinys (bendras svoris = 15,79 kg)	Pagrindo lydinys
Stiklas – šviesolaidinis, jutiklinis ekranas (bendras svoris = 0,82 kg)	Ekranas, dėžė
Varis – kabeliai (bendras svoris = 0,28 kg)	Apatinis apdorojimo blokas, ekranas, paciento jungtys
Spausdintinės plokštės (bendras svoris = 1,12 kg)	Apatinis apdorojimo blokas, ekranas, pacientų jungtys, moduliai
Pakuotė: - PE putos – 3,65 kg - Mediena – 12,98 kg - Kartonai – 6,04 kg	Pakuotė
Skysčiai/dujos	nėra
<b>Baterijos</b> , turi būti išimtos 989803169491 – (Panasonic) CGA103450A ličio jonų (12 elementų pakuotėje; 4 paketai sistemoje) Pakuotės svoris = 637,5 g 989803191341 – (BAK) 383562PN ličio polimero elementas / baterija (1 elementas pakuotėje; 3 paketai sistemoje) Pakuotės svoris = 30,2 g	Vežimėlio apatinis apdorojimo blokas  Moduliai (2 pakuotės EKG, 1 pakuotė SpO2)
Pavojinga, turi būti pašalinta: PVC PUR - 989803183221 - 989803183231	Apatinis procesoriaus vidinis vamzdelis Parduodamos NIPB prailginimo žarnelės

Patvirtinta 2015.05.19

