

Run patient samples with barcode

Patient Samples with barcode

- Select **Add sample** from **Data, Worklist:** 
- Enter the Sample ID. Cassette ID and Tube position are mandatory in case of sample without barcode.
- Select tests and dilutions from the displayed list, **Add**.
- Click on **Stat** to pipette a sample in priority.
- Click on **Low volume sample vial** if sample is in microcup.
- Select **Save sample** and continue with required samples, **Close**.
- Request a carousel hood opening by pressing on blue button in front of carousel part.
- Place sample tubes on the carousel making sure the barcode fills the slot.
- Close the carousel hood.
- Start the instrument: 



window with **OK**.

- Instrument is washing, wait for the completion of steps (SOLUTION 3 and water washing) in case of instrument power off.
- Close B·R·A·H·M·S KRYPTOR compact software: 
- Close Windows by clicking on **Start** and **Turn off**.
- Switch OFF the PC, screen, printer and instrument.

Self-determining dilution factor

Significantly reduce hands on time from sample to result

Problem

When high concentrated sample is detected out of range, it must be diluted to lower the concentration, so that the sample concentration is in the direct measuring range. Analyzers which do not have an intelligent system like self-determining dilution factor, dilution factor must be chosen manually. In addition a too high dilution should be avoided to reduce the error rate on the results. The assessment of the right dilution factor usually takes a couple of attempts. This will cost both time and material.


Solution

TRACE™ Technology used on B·R·A·H·M·S™ KRYPTOR™ has the benefit of using homogenous immunoassay and the early detection of out of range samples. As soon as the out of range sample is detected, intelligent system on B·R·A·H·M·S KRYPTOR autonomously determines the dilution factor and executes the dilution without any user intervention. This feature of self-determining dilution factor enhances the workflow.

How it works

- Step 1: Kinetic measurement method on B·R·A·H·M·S KRYPTOR is used to determine the signal increase of the analyte in the sample within few minutes.

- Step 2: If the measured relative fluorescence signal ratio of the bound and unbound signal at t_2/t_m is out of range during the first minutes of incubation, the B·R·A·H·M·S KRYPTOR will select automatically the right pre-defined dilution factor automatically and dilutes the sample.
- Step 3: Actual RFU is automatically calculated by B·R·A·H·M·S KRYPTOR after dilution.
- Step 4: RFU is then converted in concentration with the calibration curve obtained on the instrument.

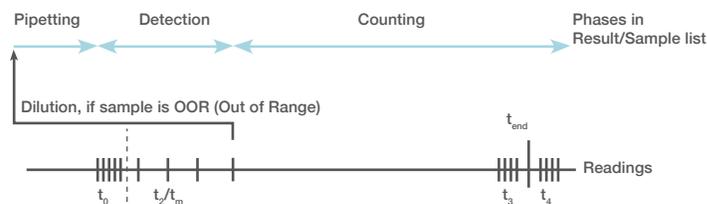

Benefits

- Easy and fast assay processing steps with TRACE Technology.
- Enhanced time to result.
- Automatic early detection of high concentrated samples to minimize/avoid hook effect.
- Optimized precision and accuracy by avoiding dilution errors.

Learn about **KRYPTOR**

Clinical Diagnostics

Thermo Fisher Scientific
B·R·A·H·M·S GmbH
Neuendorfstr. 25
16761 Hennigsdorf
Deutschland

+49 (0)3302 883 0
+49 (0)3302 883 100 Fax
info.brahms@thermofisher.com
www.thermoscientific.com/brahms



Not all products are CE marked or have 510(k) clearance for sale in the U.S.

Availability of products in each country depends on local regulatory marketing authorization status.

©2020 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified. KRYPTOR and TRACE are trademarks of Cisbio Bioassays, licensed for use by B·R·A·H·M·S GmbH, a part of Thermo Fisher Scientific. Nobel Prize is a registered trademark of the Nobel Foundation. Not all products are FDA cleared. Availability of products is related to the registration status in the countries. 901204.1

ThermoFisher
SCIENTIFIC