

PAUL HARTMANN AG
Paul-Hartmann-Strasse 12
89522 Heidenheim

Phone: +49 (0) 7321 36-0
Fax: +49 (0) 7321 36-3636
hartmann.info

P.O. Box 1420
89504 Heidenheim
Germany



Helps. Cares. Protects.

PAUL HARTMANN AG, P.O. Box 1420, 89504 Heidenheim, Germany

For the exclusive use in tender applications
(supplied either by the HARTMANN GROUP
directly or through its customer)

| | |
|----------------|----------------------------|
| Your ref. | Contact |
| - | Mrs. Laura Petran |
| Your letter of | Phone |
| - | +49 7321 36 2362 |
| Our Ref. | Fax |
| - | - |
| Date | E-Mail |
| 02.05.2023 | Laura.Petran@hartmann.info |

Confirmation

Dear Sir or Madam,

Hereby we confirm that our Foliodrape® draping materials PROTECT, PROTECT PLUS, ECO, BTC, BTC extra-reinforced, MSC and MSC extra-reinforced were tested according to EN 13795-1:2019 and fulfill all requirements of the highest possible quality level "performance level high, critical area of a product".

The conducted tests of the barrier properties follow the EN 13795-1:2019. For this highest possible quality level, it is the test according to EN ISO 22610:2006 (Resistance to microbial penetration - wet).

Tests according to EN ISO 22612:2005 (resistance to microbial penetration - dry) are not required by EN13795-1:2019 for this highest level of quality, due to the fact that it can be assumed that the requirements of EN ISO 22610:2006 (resistance to microbial penetration - wet) exceeding those of EN ISO 22612:2005.

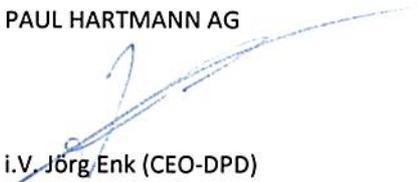
As we bring our products sterilized on the market a test for microbial cleanliness (EN 11737-1) is not necessary (see chapter 5.2 of EN 13795-1:2019):

"5.2 testing shall be performed on the finished product. If the product is to be used after sterilization, testing shall be performed on products after sterilisation with the exception of microbial cleanliness". We confirm that our products are sterile in accordance with EN 556.

Furthermore, we confirm that the total weight (mass per unit area) mentioned in our Technical data sheets is measured according to EN ISO 29073-1.

Kind regards

PAUL HARTMANN AG


i.V. Jörg Enk (CEO-DPD)


i.A. Dr. Thomas Hoffmann (CEO-RP-RD-PD-DE)

ILN 040 9500 00000 0

Vorstand/Management Board: Britta Fünfstück
(Vorsitzende des Vorstands/CEO), François Georgelin,
Stefan Grote, Stefan Müller
Aufsichtsratsvorsitzender/Chairman of the Supervisory Board:
Fritz-Jürgen Heckmann

Sitz Heidenheim
Amtsgericht Ulm HRB 661090
Registered Office Heidenheim
Commercial Register of the District Court of Ulm file no. HRB
661090