1.1. Pirkimo dalis

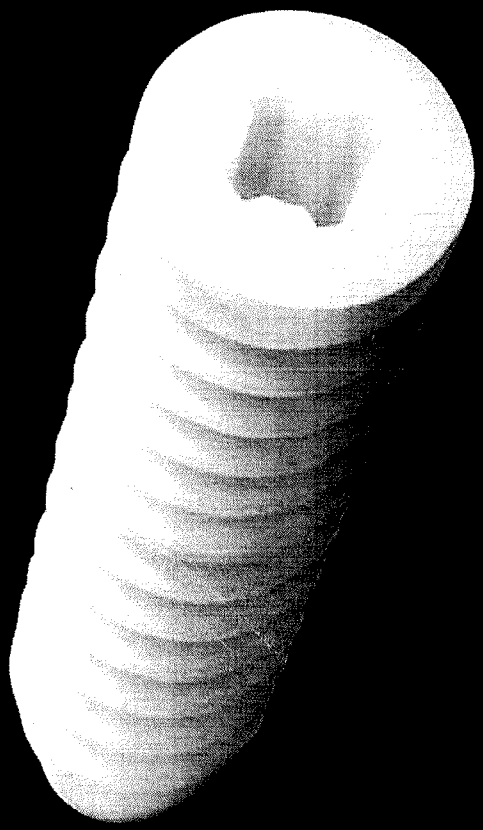

PKR interferencinės sraigtai

Our most multi-functional family of screws ever

smith&nephew

BIOSURE® HA

Interference Screw

1.1.

Sterilio je paruotije

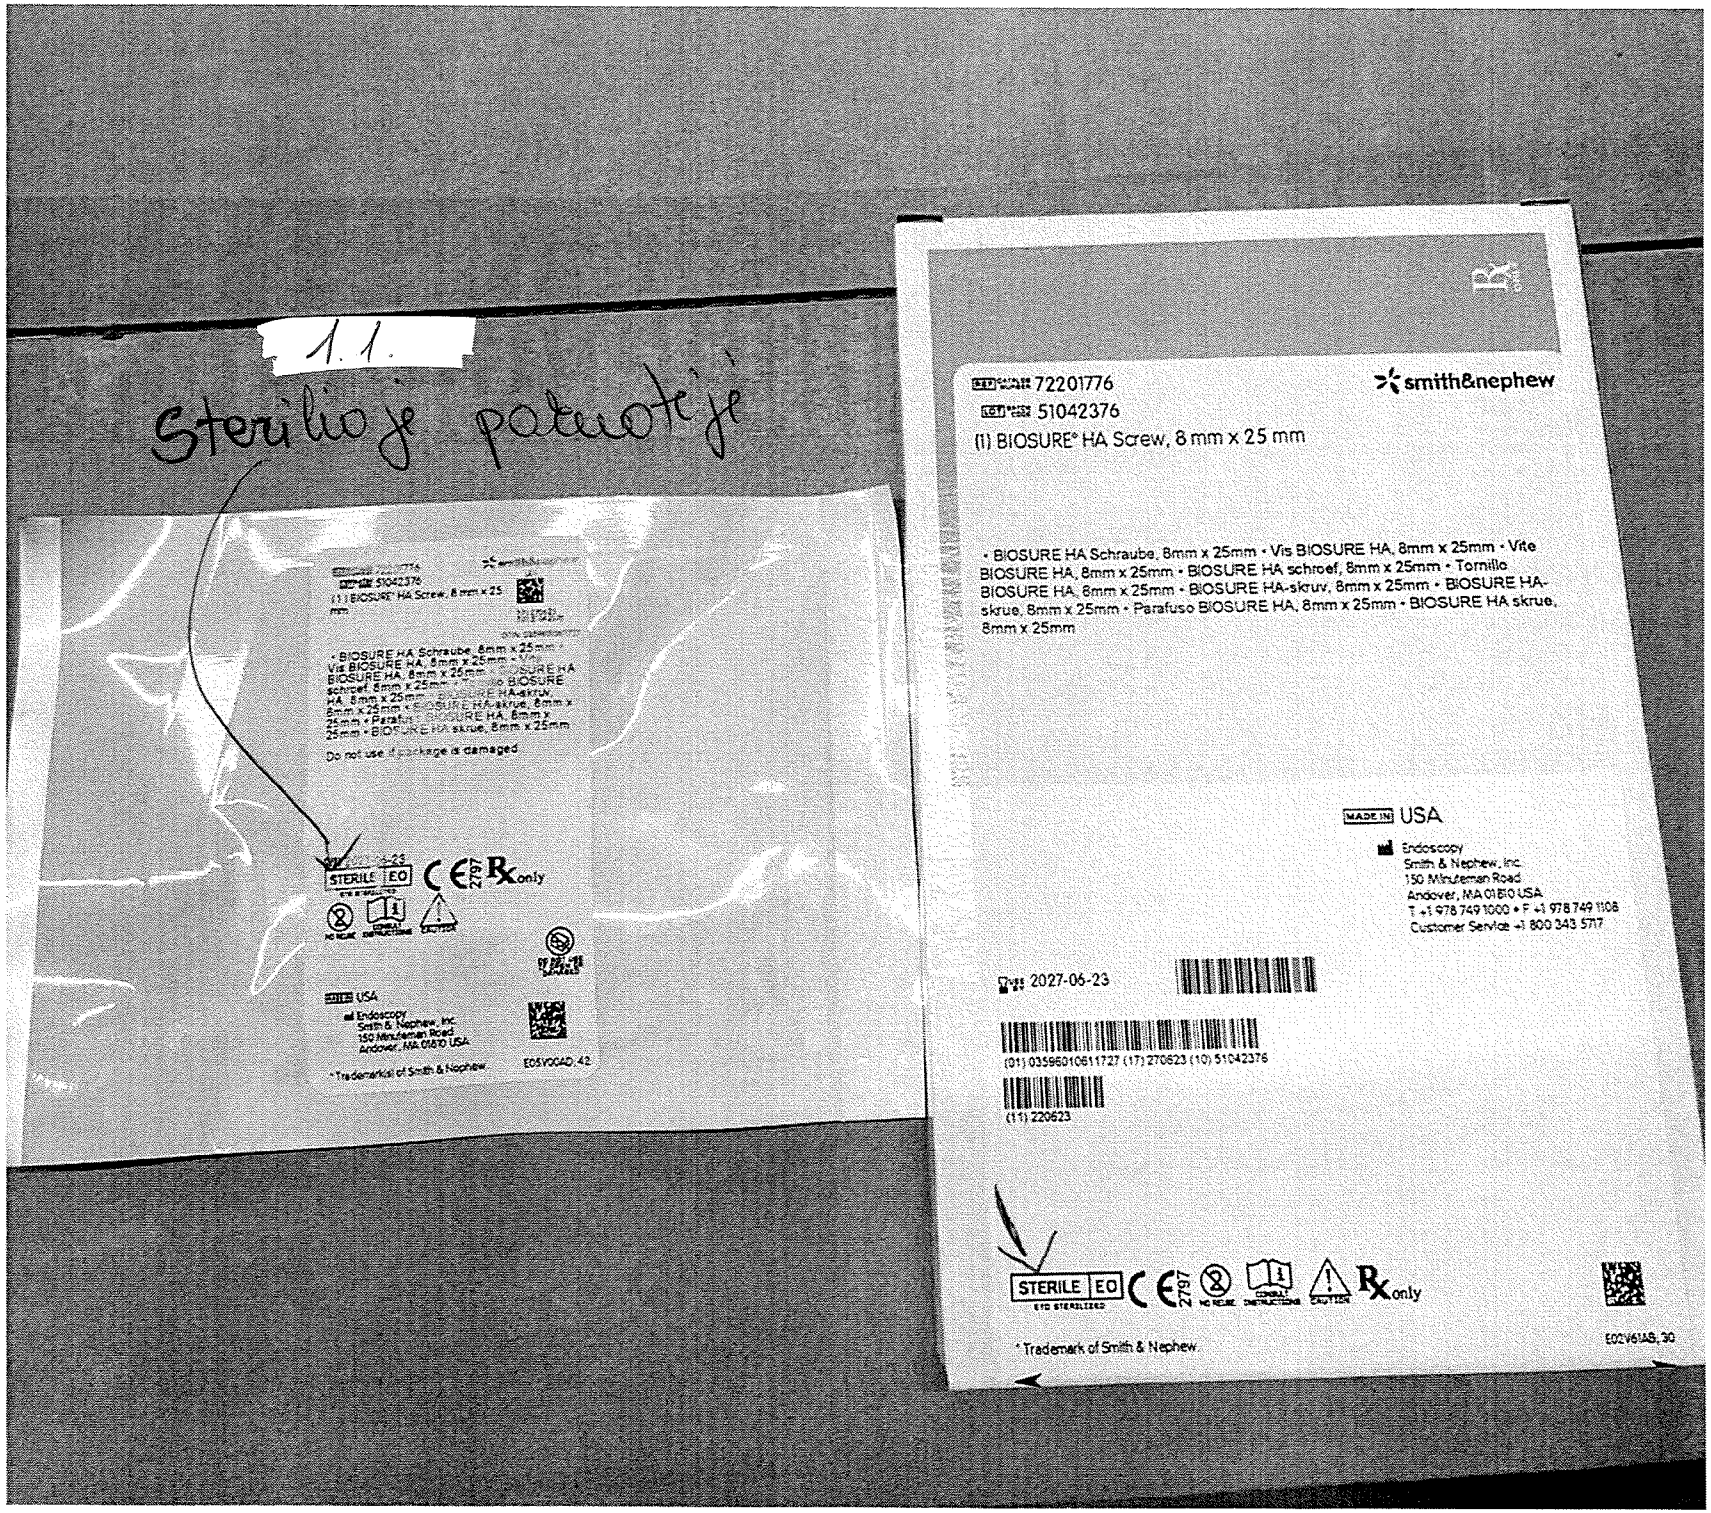

2

PKR interferenciniai sraigtai

ACL/PCL Fixation Systems

BIOSURE® HA and BIOSURE PK Interference Screws

BIOSURE Interference Screw

The BIOSURE family of interference screws provides an all-purpose range of screws and instrumentation. BIOSURE Interference Screws incorporate the latest proven technologies to help you deliver exceptional graft fixation. Available in 24 sizes, including 6 mm screws for double bundle repairs and reverse thread screws for right knees.

1.1. Besinezorb-uojantys sraigtai.

Absorbable

Our absorbable BIOSURE HA interference screw combines poly-L-lactic acid (PLLA) with hydroxyapatite (HA), a calcium phosphate similar to the mineral compound of bone. Once absorbed, it has the fracture resistance of human cortical bone. Unlike other materials where HA has been derived from animal or coralline sources, our material is completely synthetic and does not exhibit natural variability or immunological hazards.

Non-absorbable

Our non-absorbable BIOSURE PK interference screw incorporates PEEK-OPTIMA® polymer from Invibio®. Wit modulus similar to cortical bone, PEEK-OPTIMA materla exhibits an ideal combination of strength, stiffness and toughness, together with biocompatibility. BIOSURE PK interference screws offer the revisability of an absorbal screw and inherent radiolucent characteristics from a n that has gained confidence a community for 10 years.

Kopija

1.1. Sraigtų ilgiai nuo 20 - 35 mm
1.1. Sraigtų storiai nuo 6 - 12 mm.
yra didžiausio, mažiausio, tampinio storio

BIOSURE HA (PLLA-HA)

Reference #	Description
72201768	6 mm x 20 mm BIOSURE HA
72201769	6 mm x 25 mm BIOSURE HA Reversine
72201770	6 mm x 25 mm BIOSURE HA reverse thread ✓
72201771	7 mm x 20 mm BIOSURE HA
72201772	7 mm x 25 mm BIOSURE HA Reversine
72201773	7 mm x 25 mm BIOSURE HA reverse thread ✓
72201774	7 mm x 30 mm BIOSURE HA
72201775	8 mm x 20 mm BIOSURE HA
72201776	8 mm x 25 mm BIOSURE HA Reversine
72201777	8 mm x 25 mm BIOSURE HA reverse thread ✓
72201778	8 mm x 30 mm BIOSURE HA
72201779	8 mm x 35 mm BIOSURE HA
72201780	9 mm x 20 mm BIOSURE HA
72201781	9 mm x 25 mm BIOSURE HA
72201782	9 mm x 30 mm BIOSURE HA
72201783	9 mm x 35 mm BIOSURE HA
72201784	10 mm x 20 mm BIOSURE HA
72201785	10 mm x 25 mm BIOSURE HA
72201786	10 mm x 30 mm BIOSURE HA
72201787	10 mm x 35 mm BIOSURE HA
72201788	11 mm x 25 mm BIOSURE HA
72201789	11 mm x 30 mm BIOSURE HA
72201790	11 mm x 35 mm BIOSURE HA
72201791	12 mm x 35 mm BIOSURE HA

BIOSURE PK (PEEK-OPTIMA)

Reference #	Description
72202259	6 mm x 20 mm BIOSURE PK
72202260	6 mm x 25 mm BIOSURE PK
72202261	6 mm x 25 mm BIOSURE PK reverse thre
72202262	7 mm x 20 mm BIOSURE PK
72202263	7 mm x 25 mm BIOSURE PK
72202264	7 mm x 25 mm BIOSURE PK reverse thre
72202265	7 mm x 30 mm BIOSURE PK
72202266	8 mm x 20 mm BIOSURE PK
72202267	8 mm x 25 mm BIOSURE PK
72202268	8 mm x 25 mm BIOSURE PK reverse thre
72202269	8 mm x 30 mm BIOSURE PK
72202270	8 mm x 35 mm BIOSURE PK
72202271	9 mm x 20 mm BIOSURE PK
72202272	9 mm x 25 mm BIOSURE PK
72202273	9 mm x 30 mm BIOSURE PK
72202274	9 mm x 35 mm BIOSURE PK
72202275	10 mm x 20 mm BIOSURE PK
72202276	10 mm x 25 mm BIOSURE PK
72202277	10 mm x 30 mm BIOSURE PK
72202278	10 mm x 35 mm BIOSURE PK
72202279	11 mm x 25 mm BIOSURE PK
72202280	11 mm x 30 mm BIOSURE PK
72202281	11 mm x 35 mm BIOSURE PK
72202282	12 mm x 35 mm BIOSURE PK

Vertimas iš anglų kalbos

Kelio artroskopija

ACL/PCL fiksavimo sistemos

„Biosure – HA“ ir „Biosure – PK“ interferenciniai sraigtai

„BIOSURE“ interferencinis sraigtas

„Biosure“ linijos interferenciniai sraigtai turi pilną asortimentą ir instrumentariumą. „Biosure“ interferenciniai sraigtai apima naujausias įrodytas technologijas išskirtinio audinių fiksavimo srityje. Galimi 24 dydžiai, įskaitant 6 mm sraigtus dvigubai fiksacijai ir reversinio sriegio sraigtai dešinės pusės keliams.

Absorbuojami

Absorbuojami „Biosure – HA“ interferenciniai sraigtai yra poli-L-pieno rūgšties (PLLA) ir hidroksiapatito (HA) derinys, kalcio fosfatas, panašus į mineralinį kaulų junginį. Po sraigto absorbcijos, žmogaus kortikalinis kaulas įgyja atsparumą lūžiams. Skirtingai nuo kitų HA gyvulinės ar koralinės kilmės medžiagų, „Biosure“ yra pagaminti iš visiškai sintetinių medžiagų, neskatina natūralaus kintamumo ar imunologinės rizikos.

1.1. Kaniuliuoti sraigtai

Ne absorbuojami

Ne absorbuojami „Biosure PK“ interferenciniai sraigtai susideda iš „Peek Optima“ polimero iš „Invibio“. Dėl panašaus į kortikalinį kaulą modulio, „Peek Optima“ medžiaga sukuria idealų stiprumo, standumo ir kietumo derinį, kartu su biologiniu suderinamumu. „Biosure PK“ interferencinių sraigtų absorbcija ir radioliuscencinės savybės praktikoje medikų buvo stebimos jau 10 metų.

1.1. Sterilus įpakuotas su identifikacine neimenui leidžiančiu

BIOSURE HA (PLLA-HA) 1,5 mm kaniuliacija, sterilūs, 1 vnt.pakuotėje		BIOSURE PK (PEEK-OPTIMA 1,5 mm kaniuliacija, sterilūs, 1 vnt.pakuotėje	
Ref.	parametrai	Ref.	parametrai
72201768	6 mm x 20 mm BIOSURE HA	72202259	6 mm x 20 mm BIOSURE PK
72201769	6 mm x 25 mm BIOSURE HA	72202260	6 mm x 25 mm BIOSURE PK
72201770	6 mm x 25 mm BIOSURE HA reversinis sriegis	72202261	6 mm x 25 mm BIOSURE PK reversinis sriegis
72201771	7 mm x 20 mm BIOSURE HA	72202262	7 mm x 20 mm BIOSURE PK
72201772	7 mm x 25 mm BIOSURE HA	72202263	7 mm x 25 mm BIOSURE PK
72201773	7 mm x 25 mm BIOSURE HA reversinis sriegis	72202264	7 mm x 25 mm BIOSURE PK reversinis sriegis
72201774	7 mm x 30 mm BIOSURE HA	72202265	7 mm x 30 mm BIOSURE PK
72201775	8 mm x 20 mm BIOSURE HA	72202266	8 mm x 20 mm BIOSURE PK
72201776	8 mm x 25 mm BIOSURE HA	72202267	8 mm x 25 mm BIOSURE PK
72201777	8 mm x 25 mm BIOSURE HA reversinis sriegis	72202268	8 mm x 25 mm BIOSURE PK reversinis sriegis
72201778	8 mm x 30 mm BIOSURE HA	72202269	8 mm x 30 mm BIOSURE PK
72201779	8 mm x 35 mm BIOSURE HA	72202270	8 mm x 35 mm BIOSURE PK
72201780	9 mm x 20 mm BIOSURE HA	72202271	9 mm x 20 mm BIOSURE PK
72201781	9 mm x 25 mm BIOSURE HA	72202272	9 mm x 25 mm BIOSURE PK
72201782	9 mm x 30 mm BIOSURE HA	72202273	9 mm x 30 mm BIOSURE PK
72201783	9 mm x 35 mm BIOSURE HA	72202274	9 mm x 35 mm BIOSURE PK
72201784	10 mm x 20 mm BIOSURE HA	72202275	10 mm x 20 mm BIOSURE PK
72201785	10 mm x 25 mm BIOSURE HA	72202276	10 mm x 25 mm BIOSURE PK
72201786	10 mm x 30 mm BIOSURE HA	72202277	10 mm x 30 mm BIOSURE PK
72201787	10 mm x 35 mm BIOSURE HA	72202278	10 mm x 35 mm BIOSURE PK
72201788	11 mm x 25 mm BIOSURE HA	72202279	11 mm x 25 mm BIOSURE PK
72201789	11 mm x 30 mm BIOSURE HA	72202280	11 mm x 30 mm BIOSURE PK
72201790	11 mm x 35 mm BIOSURE HA	72202281	11 mm x 35 mm BIOSURE PK
72201791	12 mm x 35 mm BIOSURE HA	72202282	12 mm x 35 mm BIOSURE PK

Vertimas iš anglų kalbos

Kelio artroskopija

ACL/PCL fiksavimo sistemos

„Biosure – SYNC“ interferentiniai sraigtai

„BIOSURE- SYNC“ interferentinis sraigtas

„Biosure“ linijos interferentiniai sraigtai turi pilną asortimentą ir instrumentariumą. „Biosure“ interferentiniai sraigtai apima naujausias įrodytas technologijas išskirtinio audinių fiksavimo srityje.

Besirezorbuojantys sraigtai šlaunies raumenų sausgyslių transplanto fiksacijai. Sterilūs, kūginiai, besirezorbuojantys, sraigtas su išorine mova;

Fiksacija tribialinėje dalyje; vidutinis fiksacijos stiprumas ne mažiau 1000N;

72202744	5mm-6mm BIOSURE SYNC prietaisas
72202745	7mm-8mm BIOSURE SYNC prietaisas
72202746	9mm-10mm BIOSURE SYNC prietaisas
72202747	11mm-12mm BIOSURE SYNC prietaisas
72202843	BIOSURE SYNC instrumentų sistema

1.1. Kaniulinoti sraigtai

1.1. Pilno sriegio, su apvalia galvute.

Consistent wall thickness
Enhances screw strength.

1.1. sraigtų storiai

Sizes 6 mm to 12 mm
No ACL job is too big or too small.

Tapered design
Facilitates ease of insertion.

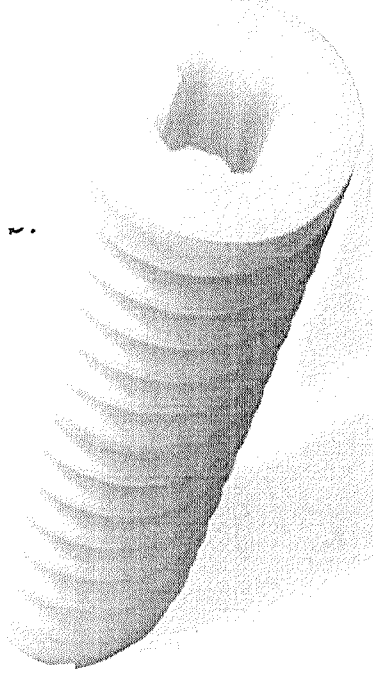

Proven Biocompatibilty
Incorporates PEEK-OPTIMA® polymer from Invibio®

1.1. **Trusted PLLA-HA material**
Gives you proven biocompatibility.
Chemine sudetis PLLA-HA.

1.1. Besirezorbuojantys sraigtai

Trusted biocompatibility

Absorbable

Our absorbable BIOSURE® HA interference screw combines poly-L-lactic acid (PLLA) with hydroxyapatite (HA), a calcium phosphate similar to the mineral compound of bone. Once absorbed, it has the fracture resistance of human cortical bone[2]. And unlike other materials where HA has been derived from animal or coralline sources, our material is completely synthetic and does not exhibit natural variability or immunological hazards.

Non-absorbable

Our non-absorbable BIOSURE PK interference screw incorporates PEEK-OPTIMA polymer from Invibio. With a modulus similar to cortical bone, PEEK-OPTIMA exhibits an ideal combination of strength, stiffness and toughness, together with biocompatibility. BIOSURE PK interference screws offer the revisability of an absorbable screw and inherent radiolucent characteristics from a material that has been gaining confidence and acceptance in the medical community for 10 years.

The right tools for easy insertion

Optimal versatility extends beyond our screw sizes. We offer a full line of instrumentation available in ratcheted or non-ratcheted versions. After all, your tools should adapt to you, not the other way around.

Innovative design
Lengthened screw well and driver improve torque and reduce breakage.



[1]Material safety data on file at Smith & Nephew
[2]Akao, M., Aoki, H. and Kato, K., Mechanical properties of sintered hydroxyapatite for prosthetic applications. Journal of Material Science: 16, 809-812, (1981)

Versatility, durability and safety[1] for all your graft fixation needs

A comprehensive solution for ACL repairs, the BIOSURE® family of interference screws and instrumentation gives you a multi-functional solution for exceptional graft fixation. Featuring the same versatility, durability, and material safety benefits as our original BIOSURE HA interference screws, non-absorbable BIOSURE PK interference screws incorporate PEEK-OPTIMA® polymer from Invibio® for proven biocompatibility.

Broadest range of sizes

Both our BIOSURE HA and BIOSURE PK interference screws are available in 24 sizes, including 6 mm screws for double bundle repairs and reverse thread screws for right knees. You'll find the ideal fit regardless of your preferred technique or patient's anatomical requirements.

Enhanced durability

All BIOSURE interference screws and drivers are desig to reduce screw breakages by optimizing stress distrit and force transfer. Both the screw well and driver have lengthened, so the driver inserts all the way to the tip. unique screw design also features a tapered body for of insertion, and a consistent wall thickness throughou added durability.

Whether you're using single or double bundle reconstruction, treating on the tibial or femoral side, using soft tissue or bone-tendon-bone grafts; choose the family of screws that overshadows the rest.

Versatility, durability and safety[1] for all your graft fixation needs

A comprehensive solution for ACL repairs, the BIOSURE◊ family of interference screws and instrumentation gives you a multi-functional solution for exceptional graft fixation. Featuring the same versatility, durability, and material safety benefits as our original BIOSURE HA interference screws, non-absorbable BIOSURE PK interference screws incorporate PEEK-OPTIMA® polymer from Invibio® for proven biocompatibility.

Broadest range of sizes

Both our BIOSURE HA and BIOSURE PK interference screws are available in 24 sizes, including 6 mm screws for double bundle repairs and reverse thread screws for right knees. You'll find the ideal fit regardless of your preferred technique or patient's anatomical requirements.

Enhanced durability

All BIOSURE interference screws and drivers are designed to reduce screw breakages by optimizing stress distribution and force transfer. Both the screw well and driver have been lengthened, so the driver inserts all the way to the tip. The unique screw design also features a tapered body for ease of insertion, and a consistent wall thickness throughout for added durability.

Whether you're doing single or double bundle reconstruction, fixating on the tibial or femoral side, using soft tissue or bone-tendon-bone grafts; choose the family of screws that overshadows the rest.

Ordering Information

BIOSURE® HA Interference Screw		BIOSURE® PK Interference Screw
72201768	6 mm x 20 mm	72202259
72201769	6 mm x 25 mm	72202260
72201770	6 mm x 25 mm, Reverse Thread	72202261
72201771	7 mm x 20 mm	72202262
72201772	7 mm x 25 mm	72202263
72201773	7 mm x 25 mm, Reverse Thread	72202264
72201774	7 mm x 30 mm	72202265
72201775	8 mm x 20 mm	72202266
72201776	8 mm x 25 mm	72202267
72201777	8 mm x 25 mm, Reverse Thread	72202268
72201778	8 mm x 30 mm	72202269
72201779	8 mm x 35 mm	72202270
72201780	9 mm x 20 mm	72202271
72201781	9 mm x 25 mm	72202272
72201782	9 mm x 30 mm	72202273
72201783	9 mm x 35 mm	72202274
72201784	10 mm x 20 mm	72202275
72201785	10 mm x 25 mm	72202276
72201786	10 mm x 30 mm	72202277
72201787	10 mm x 35 mm	72202278
72201788	11 mm x 25 mm	72202279
72201789	11 mm x 30 mm	72202280
72201790	11 mm x 35 mm	72202281
72201791	12 mm x 35 mm	72202282

Reversing 25mm ilgio

BIOSURE Tap Systems

BIOSURE Tap System	
72201889	BIOSURE Tap 6 mm
72201890	BIOSURE Tap 7 mm
72201891	BIOSURE Tap 8 mm
72201892	BIOSURE Tap 9 mm
72201893	BIOSURE Tap 10 mm
72201887	BIOSURE Driver
BIOSURE EASY TAP System	
72201190	BIOSURE EASY TAP 6 mm
72201191	BIOSURE EASY TAP 7 mm
72201192	BIOSURE EASY TAP 8 mm
72201193	BIOSURE EASY TAP 9 mm
72201194	BIOSURE EASY TAP 10 mm
72201887	BIOSURE Driver
72201888	BIOSURE Ratchet Driver
7207707	Ratcheting Handle with Hudson Adaptor

For more information, contact your local Smith & Nephew representative, or visit www.smith-nephew.com.

BIOSURE Guide Wires

7211137	Guide Wire, 1.2 mm x 9" Box of 5 Sterile
7211138	Guide Wire, 1.2 mm x 12" Box of 5 Sterile
72201201	Guide Wire, 1.2 mm x 18" Box of 5 Sterile

BIOSURE Drivers

72201887	BIOSURE Driver
72201888	BIOSURE Ratchet Driver (Requires Part Number 7207707)
7207707	Ratcheting Handle with Hudson Adaptor

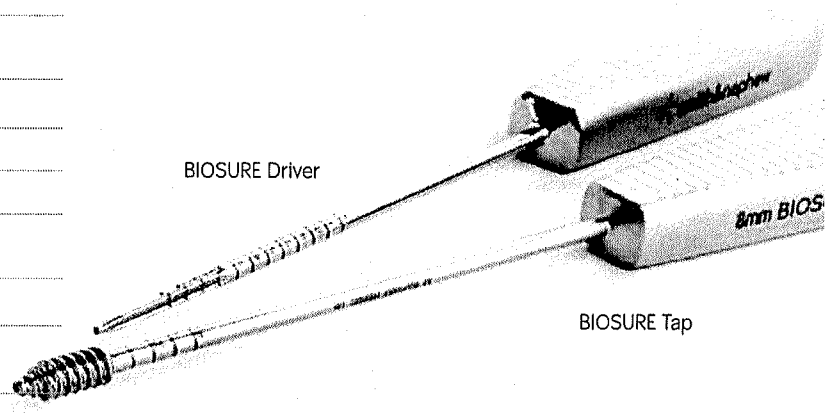

Endoscopy
Smith & Nephew, Inc.
150 Minuteman Road
Andover, MA 01810 USA

www.smith-nephew.com
T +1 978 749 1000
US Customer Service: +1 800 343 5717
International Customer Service +1 978 749 1140

*Trademark of Smith & Nephew. Certain marks Reg US Patent and Trademark Office.
©2009 Smith & Nephew, Inc. All rights reserved.
Printed in USA. 03/09 10600406 Rev. B

IORCI screws are the only nplants that offer a unique versized head incorporated nto their femoral design.

IORCI screws are optimized for urgeons utilizing the anteromedial pproach.

he enlarged head provides extra ontact area at the anatomic site. The ead also reduces any stress risers aused by "point loading" that may ccur on other full-threaded screws.

perture fixation using the BIORCI crews results in a short graft onstruct between the femoral nd tibial tunnels.

nstrumentation

o optimize the preparation of the emoral tunnel during drilling, select he RCI winged routers. These atented routers compact the nnel while drilling and provide a ountersink for the enlarged head.

Maximize your length of graft/ tunnel engagement for greater pullout strength.

BIORCI tibial-specific screws lead the industry in addressing tibial fixation issues

These longer length screws provide more soft threads to ensure maximum length interference between the graft and tibial tunnel.

Designed in conjunction with leading surgeons to maximize the fixation along the tibial tunnel.

Instrumentation

The tibial tunnel can be prepared with either the RCI tibial compaction routers or a standard cannulated drill bit.

padidinta polunti

BIORCI screws with a rounded head and soft threads for maximum protection of the grafts.

The latest addition to the RCI screw line.

Femoral screws with a matched rounded head. These screws incorporate the same Torx® interface as all BIORCI screws to minimize breakage when your approach is through the tibial tunnel.

The 1.5 mm guide wire is the largest in the industry to assist you in accurate parallel placement of the screws.

Instrumentation

The transtibial approach utilizes an endoscopic cannulated drill bit for femoral tunnel preparation and a cannulated drill bit for drilling the tibial tunnel.

reversinis srigaia

Reverse Thread – because your patients do not have two left knees.

Use the patented Reverse Thread BIORCI bioabsorbable screw for your right knees.

To produce mirror images on right and left limbs, the final femoral graft position within the tunnel must be the same.

Standard (clockwise) screw thread orientation produces clockwise rotation of the graft in left knees, resulting in a posterior final graft position. However, standard (clockwise) screw thread orientation results in an anterior final femoral graft position within the femoral tunnel in right knees.

Therefore, to achieve a posterior final graft position in a right knee, to mirror the rotation of the left knee, a reverse (counterclockwise) threaded screw may be selected.

Instrumentation

To optimize the preparation of the femoral tunnel during drilling, select the RCI winged routers.

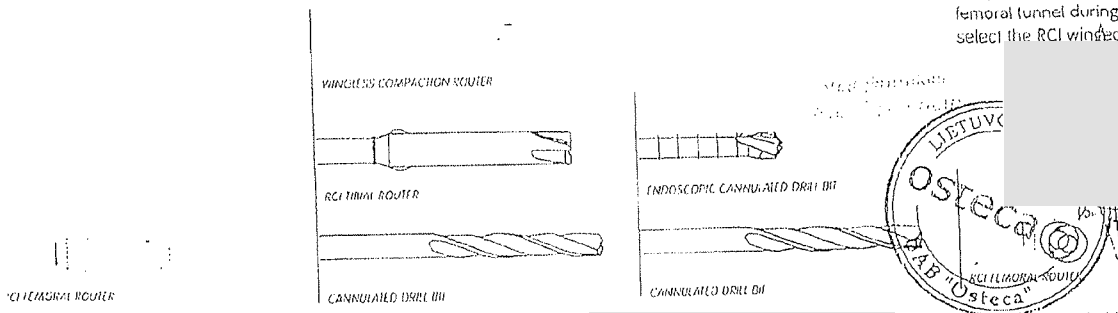

LIETUVO Osteca TAB "Osteca"

o maximize product efficiency it is recommended that the surgical site is pre[redacted] to insertion of the absorbable implant.

- 30 Kopija tikra

ACL/PCL Fixation Systems

BIORCI® Screws

↑

su padidinta galvute

BIORCI Screws

PLLA Bioabsorbable Interference Screws, 1.5 mm cannulation, blunt threads. Standard and enlarged heads. Sterile, 1 per box.

kanuliacija / bukas sriegis

Reference #	Description
7207916	7 x 20 mm BIORCI Screw
7207554*	7 x 25 mm BIORCI Screw
7207607	7 x 25 mm BIORCI Screw with an 8 mm head reverse thread
7207555	7 x 30 mm BIORCI Screw
7207557	7 x 25 mm BIORCI Screw with an 8 mm head
7207558	7 x 30 mm BIORCI Screw with an 8 mm head
7207918	8 x 20 mm BIORCI Screw
7207560	8 x 25 mm BIORCI Screw
7207608*	8 x 25 mm BIORCI Screw reverse thread
7207561	8 x 30 mm BIORCI Screw
7207562	8 x 35 mm BIORCI Screw
7207919	9 x 20 mm BIORCI Screw
7207563	9 x 25 mm BIORCI Screw
7207924	9 x 25 mm BIORCI Screw reverse thread
7207564	9 x 30 mm BIORCI Screw
7207565	9 x 35 mm BIORCI Screw
7207566	10 x 25 mm BIORCI Screw
7207581	10 x 25 mm BIORCI Screw reverse thread
7207567	10 x 30 mm BIORCI Screw
7207568*	10 x 35 mm BIORCI Screw
7207920	11 x 30 mm BIORCI Screw
7207921	11 x 35 mm BIORCI Screw
7207923	12 x 35 mm BIORCI Screw

1.1. Reversinė su padidinta galvute.

* Item shown

Special, Made to Order products are available to meet the individual needs of surgeons. Please appreciate that longer lead time for delivery should be expected. For more information, please contact your sales representative or Customer Service.

Vertimas iš anglų kalbos

Užsakymo informacija
Smith&Nephew siūlo viską ko reikia kryžminių raiščių rekonstrukcijoms – nuo bioabsorbcinių sraigtų iki instrumentų.

Biorci sraigtų sistemos implantai
1,5 mm kaniuliacija, sterilūs, dėžutėje 1 vnt.

7207554	Sraigtas BIORCI 7 mm(7 mm x25mm)
7207555	Sraigtas BIORCI 7 mm(7 mm x30mm)
7207557	Sraigtas BIORCI 7 mm(8 mm x25mm)
7207558	Sraigtas BIORCI 7 mm(8 mm x30mm)
7207560	Sraigtas BIORCI 8 x 25 mm
7207561	Sraigtas BIORCI 8 x 30 mm
7207562	Sraigtas BIORCI 8 x 35 mm
7207563	Sraigtas BIORCI 9 x 25 mm
7207564	Sraigtas BIORCI 9 x 30 mm
7207565	Sraigtas BIORCI 9 x 35 mm
7207567	Sraigtas BIORCI 10 x 30 mm
7207568	Sraigtas BIORCI 10 x 35 mm
7207607	Sraigtas BIORCI 7 mm (8 mm x 25 mm reversiniu sreigiu)
7207608	Sraigtas BIORCI 8 x 25 mm reversiniu sriegiu

Biorci-HA sraigtai
1,5 mm kaniuliacija, sterilūs, dėžutėje 1 vnt.

7207686	BIORCI-HA 7/7 x 20 mm
7207674	BIORCI-HA 7/7 x 25 mm
7207677	BIORCI-HA 7/7 x 30 mm
7207675	BIORCI-HA 7/8 x 25 mm
7207676	BIORCI-HA 7/8 x 30 mm
7209012	BIORCI-HA 8 x 20 mm
7207678	BIORCI-HA 8 x 25 mm
7207679	BIORCI-HA 8 x 30 mm
7207680	BIORCI-HA 8 x 35 mm
7209013	BIORCI-HA 9 x 20 mm
7207681	BIORCI-HA 9 x 25 mm
7207682	BIORCI-HA 9 x 30 mm
7207683	BIORCI-HA 9 x 35 mm
7209016	BIORCI-HA 10 x 25 mm
7209017	BIORCI-HA 10 x 30 mm
7209018	BIORCI-HA 10 x 35 mm
7209014	BIORCI-HA 11 x 30 mm
7209022	BIORCI-HA 11 x 35 mm
7209015	BIORCI-HA 12 x 35 mm
7209023	BIORCI-HA 7/8 x 25 mm, reversinė
7209021	BIORCI-HA 8 x 25 mm, reversinė
7209020	BIORCI-HA 9 x 25 mm, reversinė
7209019	BIORCI-HA 10 x 25 mm, reversinė
7207636	1.5 mm x 9" (23 cm) pravedėjas
014859	1.5 mm x 12" (30 cm) pravedėjas
3134033	1.5 mm x 17" (30 cm) pravedėjas

LIETUVOS RESPUBLIKA UAB "Osteca" KRETINGA

Kopija tikra

1.1. sterilus sporavimas, su identifikavimo numeriu.

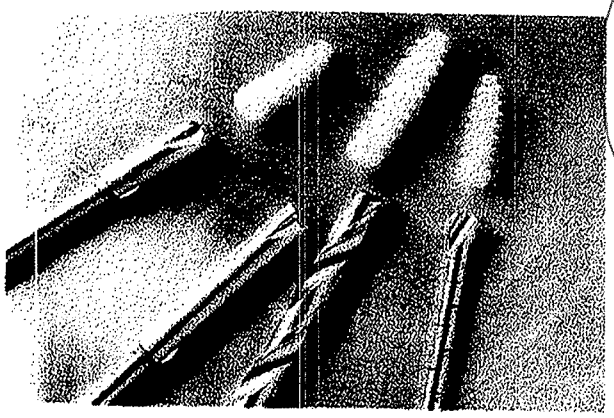

Ordering Information

From bioabsorbable screws to powered instrumentation, Smith & Nephew offers everyth need for consistently strong cruciate reconstructions.

3.1.1. standartine su paddinta galute.

BIORCI Screw System Implants

1.5 mm cannulation, sterile, 1 per box

7207554	Screw, BIORCI 7 mm (7 mm Head) x 25 mm
7207555	Screw, BIORCI 7 mm (7 mm Head) x 30 mm
7207557	Screw, BIORCI 7 mm (8 mm Head) x 25 mm
7207558	Screw, BIORCI 7mm (8 mm Head) x 30 mm
7207560	Screw, BIORCI 8 x 25 mm
7207561	Screw, BIORCI 8 x 30 mm
7207562	Screw, BIORCI 8 x 35 mm
7207563	Screw, BIORCI 9 x 25 mm
7207564	Screw, BIORCI 9 x 30 mm
7207565	Screw, BIORCI 9 x 35 mm
7207567	Screw, BIORCI 10 x 30 mm
7207568	Screw, BIORCI 10 x 35 mm
7207607	Screw, BIORCI 7mm (8 mm x 25 mm, Reverse Thread
7207608	Screw, BIORCI 8 x 25 mm, Reverse Thread

1.1. kanulinioti sterilus

BIORCI-HA Screws

1.5 mm cannulation, sterile, 1 per box

7207686	Screw, BIORCI-HA 7/7 x 20 mm
7207674	Screw, BIORCI-HA 7/7 x 25 mm
7207677	Screw, BIORCI-HA 7/7 x 30 mm
7207675	Screw, BIORCI-HA 7/8 x 25 mm
7207676	Screw, BIORCI-HA 7/8 x 30 mm
7209012	Screw, BIORCI-HA 8 x 20 mm
7207678	Screw, BIORCI-HA 8 x 25 mm
7207679	Screw, BIORCI-HA 8 x 30 mm
7207680	Screw, BIORCI-HA 8 x 35 mm
7209013	Screw, BIORCI-HA 9 x 20 mm
7207681	Screw, BIORCI-HA 9 x 25 mm
7207682	Screw, BIORCI-HA 9 x 30 mm
7207683	Screw, BIORCI-HA 9 x 35 mm
7209016	Screw, BIORCI-HA 10 x 25 mm
7209017	Screw, BIORCI-HA 10 x 30 mm
7209018	Screw, BIORCI-HA 10 x 35
7209014	Screw, BIORCI-HA 11 x 30
7209022	Screw, BIORCI-HA 11 x 35
7209015	Screw, BIORCI-HA 12 x 35
7209023	Screw, BIORCI-HA 7/8 x 25 Reverse Thread
7209021	Screw, BIORCI-HA 8 x 25 r Reverse Thread
7209020	Screw, BIORCI-HA 9 x 25 r Reverse Thread
7209019	Screw, BIORCI-HA 10 x 25 Reverse Thread
7207636	1.5 mm x 9" (23 cm) Guide
014859	1.5 mm x 12" (30 cm) Guic
3134033	1.5 mm x 17" (30 cm) Guic

BIORCI-HA Screw System Instrumentation

7208661	7 mm BIORCI Tap
7208662	8 mm BIORCI Tap
7208663	9 mm BIORCI Tap
7208664	10 mm BIORCI Tap
7208656	BIORCI Torx® Driver
7207359	BIORCI Starter
7207369	BIORCI Tray
7207766	Wingless Compaction Rout
3134186	Single Flute Endoscopic Dri

Kopija tikra

LIETUVOS RESPUBLIKA UAB "Osteca" KRETINGA

BIORCI Absorbable Screws offer optimal strength and selection for soft tissue and B-T-B reconstructions.



*Pullout Strength Chart comparing BIORCI strength of fixation vs. competitors. BIORCI bioabsorbable screw is 28% more effective at maintaining fixation than the closest competitor.***



*Comparison chart showing a 58% increase in tibial pullout strength utilizing longer length screws.***

[1] *C.M.Agrawal, M. Fan, C. Zhu and K.A. Athanasiou: A New Technique to Control the pH in the Vicinity of Bioabsorbable Implants.*

* In vitro data on file with Smith & Nephew. ** Data on file with Smith & Nephew.

Complete BIORCI Screw Systems can be tailored to include guides, manual and powered instrumentati Ask your local sales representative for assistance.

Endoscopy
Smith & Nephew, Inc.
Andover MA 01810
USA

www.smith-nephew.com
T +1 978 749 1000
F +1 978 749 1108
US Customer Service +1 800 343 5717

BIORCI is a trademark of Smith & Nephew, Inc. Reg US Pat & TM Off.
Torx is a registered trademark of Textron, Inc.
©2001, 2002, 2007 Smith & Nephew, Inc. All rights reserved. Printed in USA.

09/07 10600331 F

Vertimas iš anglų kalbos

Kelio artroskopija A-12

ACL/PCL fiksavimo sistemos

BIORCI – HA sraigtai

BIORCI-HA sraigtų sistemos implantai

BIORCI-HA sraigtų sistemos yra efektyvios fiksuojant transplantantus. BIORCI-HA sraigtams yra naudojami standartiniai BIORCI instrumentai; 23 sraigtų dydžiai.

1.1. su padidinta galvute. 7/8

Ref	Parametrai
7207686	BIORCI-HA 7/7 x 20 mm
7207674	BIORCI-HA 7/7 x 25 mm
7207677	BIORCI-HA 7/7 x 30 mm
7207675	BIORCI-HA 7/8 x 25 mm ✓
7207676	BIORCI-HA 7/8 x 30 mm ✓
7209012	BIORCI-HA 8 x 20 mm
7207678	BIORCI-HA 8 x 25 mm
7207679	BIORCI-HA 8 x 30 mm
7207680	BIORCI-HA 8 x 35 mm
7209013	BIORCI-HA 9 x 20 mm
7207681	BIORCI-HA 9 x 25 mm
7207682	BIORCI-HA 9 x 30 mm
7207683	BIORCI-HA 9 x 35 mm
7209016	BIORCI-HA 10 x 25 mm
7209017	BIORCI-HA 10 x 30 mm
7209018	BIORCI-HA 10 x 35 mm
7209014	BIORCI-HA 11 x 30 mm
7209022	BIORCI-HA 11 x 35 mm
7209015	BIORCI-HA 12 x 35 mm
7209023	BIORCI-HA 7/8 x 25 mm, reversinė
7209021	BIORCI-HA 8 x 25 mm, reversinė
7209020	BIORCI-HA 9 x 25 mm, reversinė
7209019	BIORCI-HA 10 x 25 mm, reversinė
7207636	1.5 mm x 9" (23 cm) pravedėjas, nesterilus, pakuotėje 6 vnt.
014859	1.5 mm x 12" (30 cm) pravedėjas, nesterilus, pakuotėje 1 vnt.

1.1. Daugiau nei 3 dydžių.

1.1. Reversinis sriegis su padidinta galvute

1.1. Biorci Ha sraigtai yra pagaminti iš 80% PLLA ir 20% hydroksilapatito (HA) geresniam absorbavimui. Implantavimo vietoje HA padeda kontroliuoti pH. HA yra sumaišytas su PLLA ilgesniam HA išliekamumui absorbavimo proceso metu.

LIETUVOS RESPUBLIKA UAB "Osteca" KRETINGA

Kopija tikra

[redacted]

14

ACL/PCL Fixation Systems

BIORCI®-HA Screws

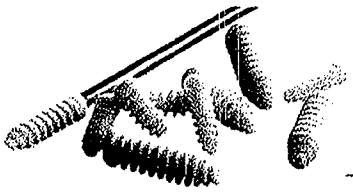

BIORCI-HA Screw System Implants

The BIORCI–HA Screw System has proven effectiveness for graft fixation and site repair. BIORCI-HA screws use standard BIORCI instruments and offer 23 screw sizes from which to choose.

Reference #	Description
7207686	7/7 x 20 mm BIORCI-HA
7207674	7/7 x 25 mm BIORCI-HA
7207677	7/7 x 30 mm BIORCI-HA
7207675	7/8 x 25 mm BIORCI-HA
7209023	7/8 x 25 mm BIORCI-HA reverse thread
7207676	7/8 x 30 mm BIORCI-HA
7209012	8 x 20 mm BIORCI-HA
7207678	8 x 25 mm BIORCI-HA
7209021	8 x 25 mm BIORCI-HA reverse thread
7207679	8 x 30 mm BIORCI-HA
7207680	8 x 35 mm BIORCI-HA
7209013	9 x 20 mm BIORCI-HA
7207681	9 x 25 mm BIORCI-HA
7209020	9 x 25 mm BIORCI-HA reverse thread
7207682	9 x 30 mm BIORCI-HA
7207683	9 x 35 mm BIORCI-HA
7209016	10 x 25 mm BIORCI-HA
7209019	10 x 25 mm BIORCI-HA reverse thread
7209017	10 x 30 mm BIORCI-HA
7209018	10 x 35 mm BIORCI-HA
7209014	11 x 30 mm BIORCI-HA
7209022	11 x 35 mm BIORCI-HA
7209015	12 x 35 mm BIORCI-HA
7207636	1.5 mm x 9" (23 cm) Guide Wire, non-sterile (6 per package)
014859	1.5 mm x 12" (30 cm) Guide Wire, sterile (1 per package)

1.1.

Reversine

LIETUVOS RESPUBLIKA UAB "Osteca" KRETING

Kopija tikra

15

1.1.

Nadidinde palonte

1.1.

reversinis vitgis

IORCI screws are the only nplants that offer a unique versized head incorporated nto their femoral design.

IORCI screws are optimized for urgeons utilizing the anteromedial pproach.

he enlarged head provides extra ontact area at the anatomic site. The ead also reduces any stress risers eused by "point loading" that may ccur on other full-threaded screws.

perture fixation using the BIORCI crews results in a short graft onstruct between the femoral nd tibial tunnels.

nstrumentation

o optimize the preparation of the emoral tunnel during drilling, select ne RCI winged routers. These atented routers compact the nnel while drilling and provide a ountersink for the enlarged head.

Maximize your length of graft/ tunnel engagement for greater pullout strength.

BIORCI tibial-specific screws lead the industry in addressing tibial fixation issues.

These longer length screws provide more soft threads to ensure maximum length interference between the graft and tibial tunnel.

Designed in conjunction with leading surgeons to maximize the fixation along the tibial tunnel.

Instrumentation

The tibial tunnel can be prepared with either the RCI tibial compaction routers or a standard cannulated drill bit.

BIORCI screws with a rounded head and soft threads for maximum protection of the grafts.

The latest addition to the RCI screw line.

Femoral screws with a matched rounded head. These screws incorporate the same Torx® interface as all BIORCI screws to minimize breakage when your approach is through the tibial tunnel.

The 1.5 mm guide wire is the largest in the industry to assist you in accurate parallel placement of the screws

Instrumentation

The transtibial approach utilizes an endoscopic cannulated drill bit for femoral tunnel preparation and a cannulated drill bit for drilling the tibial tunnel.

Reverse Thread – because your patients do not have two left knees.

Use the patented Reverse Thread BIORCI bioabsorbable screw for your right knees.

To produce mirror images on right and left limbs, the final femoral graft position within the tunnel must be the same.

Standard (clockwise) screw thread orientation produces clockwise rotation of the graft in left knees, resulting in a posterior final graft position. However, standard (clockwise) screw thread orientation results in an anterior final femoral graft position within the femoral tunnel in right knees.

Therefore, to achieve a posterior final graft position in a right knee, to mirror the rotation of the left knee, a reverse (counterclockwise) threaded screw may be selected.

Instrumentation

To optimize the preparation of the femoral tunnel during drilling, select the RCI winged routers.

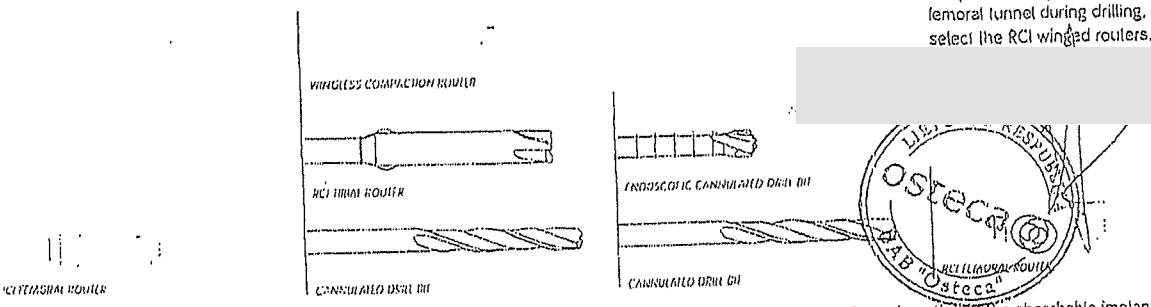

o maximize product efficiency it is recommended that the surgical site is [redacted] with the BIORCI Starter or Tap prior to insertion of the absorbable implant.

[redacted]

5-11-30 Kopija tikra

Developed by Smith & Nephew, BIORCI® Bioabsorbable Interference Screws are among the strongest bioabsorbable screws available for arthroscopists performing soft tissue or bone-tendon-bone (B-T-B) reconstructions. With one of the highest pull-out strengths and the greatest resistance to breakage among bioabsorbable screws, BIORCI® Screws are designed to hold the graft in place for secure anatomic aperture reconstruction. BIORCI-HA® Screws go a step further, combining the proven strength and integrity of the BIORCI Screw System with hydroxylapatite (HA).

BIORCI® and BIORCI®-HA

Enhanced Bioabsorbable Screws

BIORCI and BIORCI-HA bioabsorbable screws are a complete line of bioabsorbable implants allowing for multiple approaches of repair and the flexibility to accommodate a variety of anatomical placements.

Longer thread engagement provides greater pullout strength within the tibial tunnel.

Unique Torx® interface helps minimize breakage

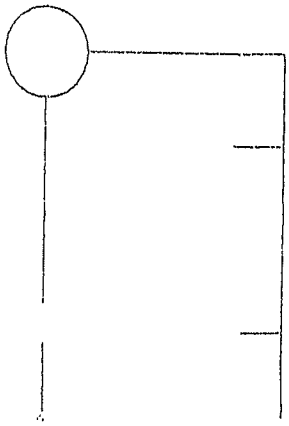

BIORCI bioabsorbable screw is the only system that includes reverse-threaded screws to keep the soft tissue grafts in optimal position.

Unique and patented Torx driver-to-screw interface disperses force throughout the screw during insertion.

Smith & Nephew is the developer of the first soft tissue fixation screw. We offer the broadest choice in technique-specific screws today, with quality and reliability second to none.

A safe, proven alternative to metal screws, BIORCI-HA screws are strong when needed, then absorb discreetly.

Research indicates the pH levels surrounding the absorption of polymers is reduced with the combined absorption of hydroxylapatite.[1]

Laser markings ensure that implants are fully sealed

BIORCI-HA screws offer 20 mm and 25 mm lengths for use with bone-tendon-bone grafts.

The 20 mm and 25 mm length screws are sized for optimal bone-tendon-bon graft fixation. Soft threads minimize gra laceration, and range of diameters ens a tight fit in all tunnels.

Instrumentation

The bone-tendon-bone approach utilizes an endoscopic cannulated drill bit for femoral tunnel preparation and a cannulated drill bit for drilling the tibial tunnel.



ENDOSCOPIC CANNULATED DRILL BIT

CANNULATED DRILL BIT

LIETUVOS RESPUBLIKA
Osteca
UAB "Osteca"
Kopija tikra

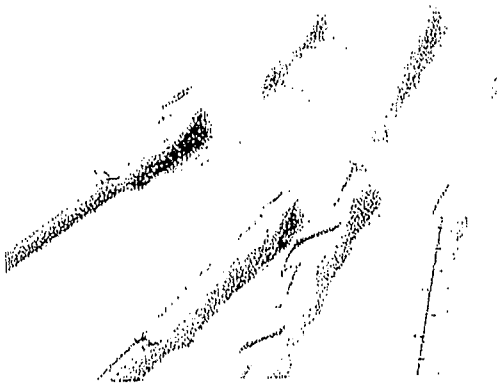

BIORCI Absorbable Screws offer optimal strength and selection for soft tissue and B-T-B reconstructions.

*Pullout Strength Chart comparing BIORCI strength of fixation vs. competitors. BIORCI bioabsorbable screw is 28% more effective at maintaining fixation than the closest competitor.**

*Comparison chart showing a 58% increase in tibial pullout strength utilizing longer length screws.**

[1] *C.M Agrawal, M. Fan, C. Zhu and K.A. Athanasiou. A New Technique to Control the pH in the Vicinity of Bioabsorbable Implants.*

* In vitro data on file with Smith & Nephew. ** Data on file with Smith & Nephew

Ordering Information

From bioabsorbable screws to powered instrumentation, Smith & Nephew offers e
need for consistently strong cruciate reconstructions.

BIORCI Screw System Implants

1.5 mm cannulation, sterile, 1 per box

7207554	Screw, BIORCI 7 mm (7 mm Head) x 25 mm
7207555	Screw, BIORCI 7 mm (7 mm Head) x 30 mm
7207557	Screw, BIORCI 7 mm (8 mm Head) x 25 mm
7207558	Screw, BIORCI 7mm (8 mm Head) x 30 mm
7207560	Screw, BIORCI 8 x 25 mm
7207561	Screw, BIORCI 8 x 30 mm
7207562	Screw, BIORCI 8 x 35 mm
7207563	Screw, BIORCI 9 x 25 mm
7207564	Screw, BIORCI 9 x 30
7207565	Screw, BIORCI 9 x 35
7207567	Screw, BIORCI 10 x 3
7207568	Screw, BIORCI 10 x 3
7207607	Screw, BIORCI 7mm (x 25 mm, Reverse Th
7207608	Screw, BIORCI 8 x 25 Reverse Thread

4. 1.

Sterile.

BIORCI-HA Screws

1.5 mm cannulation, sterile, 1 per box

7207686	Screw, BIORCI-HA 7/7 x 20 mm
7207674	Screw, BIORCI-HA 7/7 x 25 mm
7207677	Screw, BIORCI-HA 7/7 x 30 mm
7207675	Screw, BIORCI-HA 7/8 x 25 mm
7207676	Screw, BIORCI-HA 7/8 x 30 mm
7209012	Screw, BIORCI-HA 8 x 20 mm
7207678	Screw, BIORCI-HA 8 x 25 mm
7207679	Screw, BIORCI-HA 8 x 30 mm
7207680	Screw, BIORCI-HA 8 x 35 mm
7209013	Screw, BIORCI-HA 9 x 20 mm
7207681	Screw, BIORCI-HA 9 x 25 mm
7207682	Screw, BIORCI-HA 9 x 30 mm
7207683	Screw, BIORCI-HA 9 x 35 mm
7209016	Screw, BIORCI-HA 10 x 25 mm
7209017	Screw, BIORCI-HA 10 x 30 mm
7209018	Screw, BIORCI-HA 1(
7209014	Screw, BIORCI-HA 1
7209022	Screw, BIORCI-HA 1
7209015	Screw, BIORCI-HA 1
7209023	Screw, BIORCI-HA 7/ Reverse Thread
7209021	Screw, BIORCI-HA 8 Reverse Thread
7209020	Screw, BIORCI-HA 9 Reverse Thread
7209019	Screw, BIORCI-HA 1(Reverse Thread
7207636	1.5 mm x 9" (23 cm)
014859	1.5 mm x 12" (30 cm
3134033	1.5 mm x 17" (30 cm

BIORCI-HA Screw System Instrumentation

7208661	7 mm BIORCI Tap
7208662	8 mm BIORCI Tap
7208663	9 mm BIORCI Tap
7208664	10 mm BIORCI Tap
7208656	BIORCI Torx** Driver
7207359	BIORCI Starter
7207369	BIORCI Tray
7207766	Wingless Compactio
3134186	Single Flute Endosco

LIETUVOS K
Osteo
UAB "Osteo"

Complete BIORCI Screw Systems can be tailored to include guides, manual and powered instr
Ask your local sales representative for assistance.

Endoscopy
Smith & Nephew, Inc.
Andover MA 01810
USA

www.smith-nephew.com
T +1 978 749 1000
F +1 978 749 1108
US Customer Service +1 800 343 5717

BIORCI is a trademark of Smith & Nephew, Inc. Reg US Pat & TM Off
Torx is a registered trademark of Textron, Inc
©2001, 2002, 2007 Smith & Nephew, Inc. All rights reserved. Printed in USA.

09/07 10

1.2 Pirkimo dalis

Everything ultra in cortical fixation.

The ULTRABUTTON® Adjustable Fixation Device provides leading strength and displacement properties[1] while also incorporating a unique cradle design to help protect the graft during loop reduction.

Endosaga su savaime užsiveržiančia kilpa.

Graft Cradle

- Designed to protect graft with large contact area
- Designed to reduce relative motion and sawing effect between device and graft

Interlocking Adjustment

- Maximizes graft in tunnel
- Requires minimal force to reduce loop

Skirta šlauninės pusės fiksacijai

One-handed Adjustment

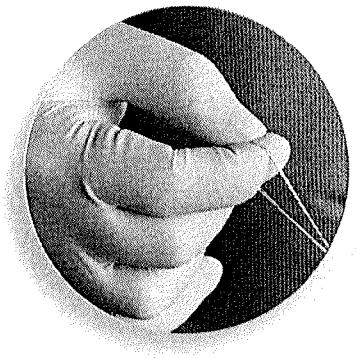

Finger Loop

- Facilitates convenient one-handed reduction
- Enables user to do both reduction and counter-tensioning

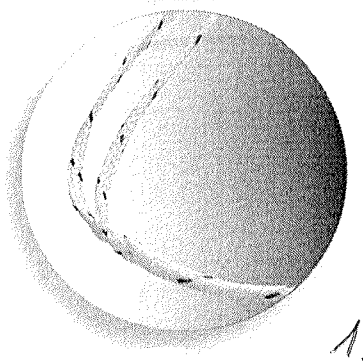

Tail Bridge

- Provides one-handed adjustment
- Helps ensure uniform graft ascension into tunnel

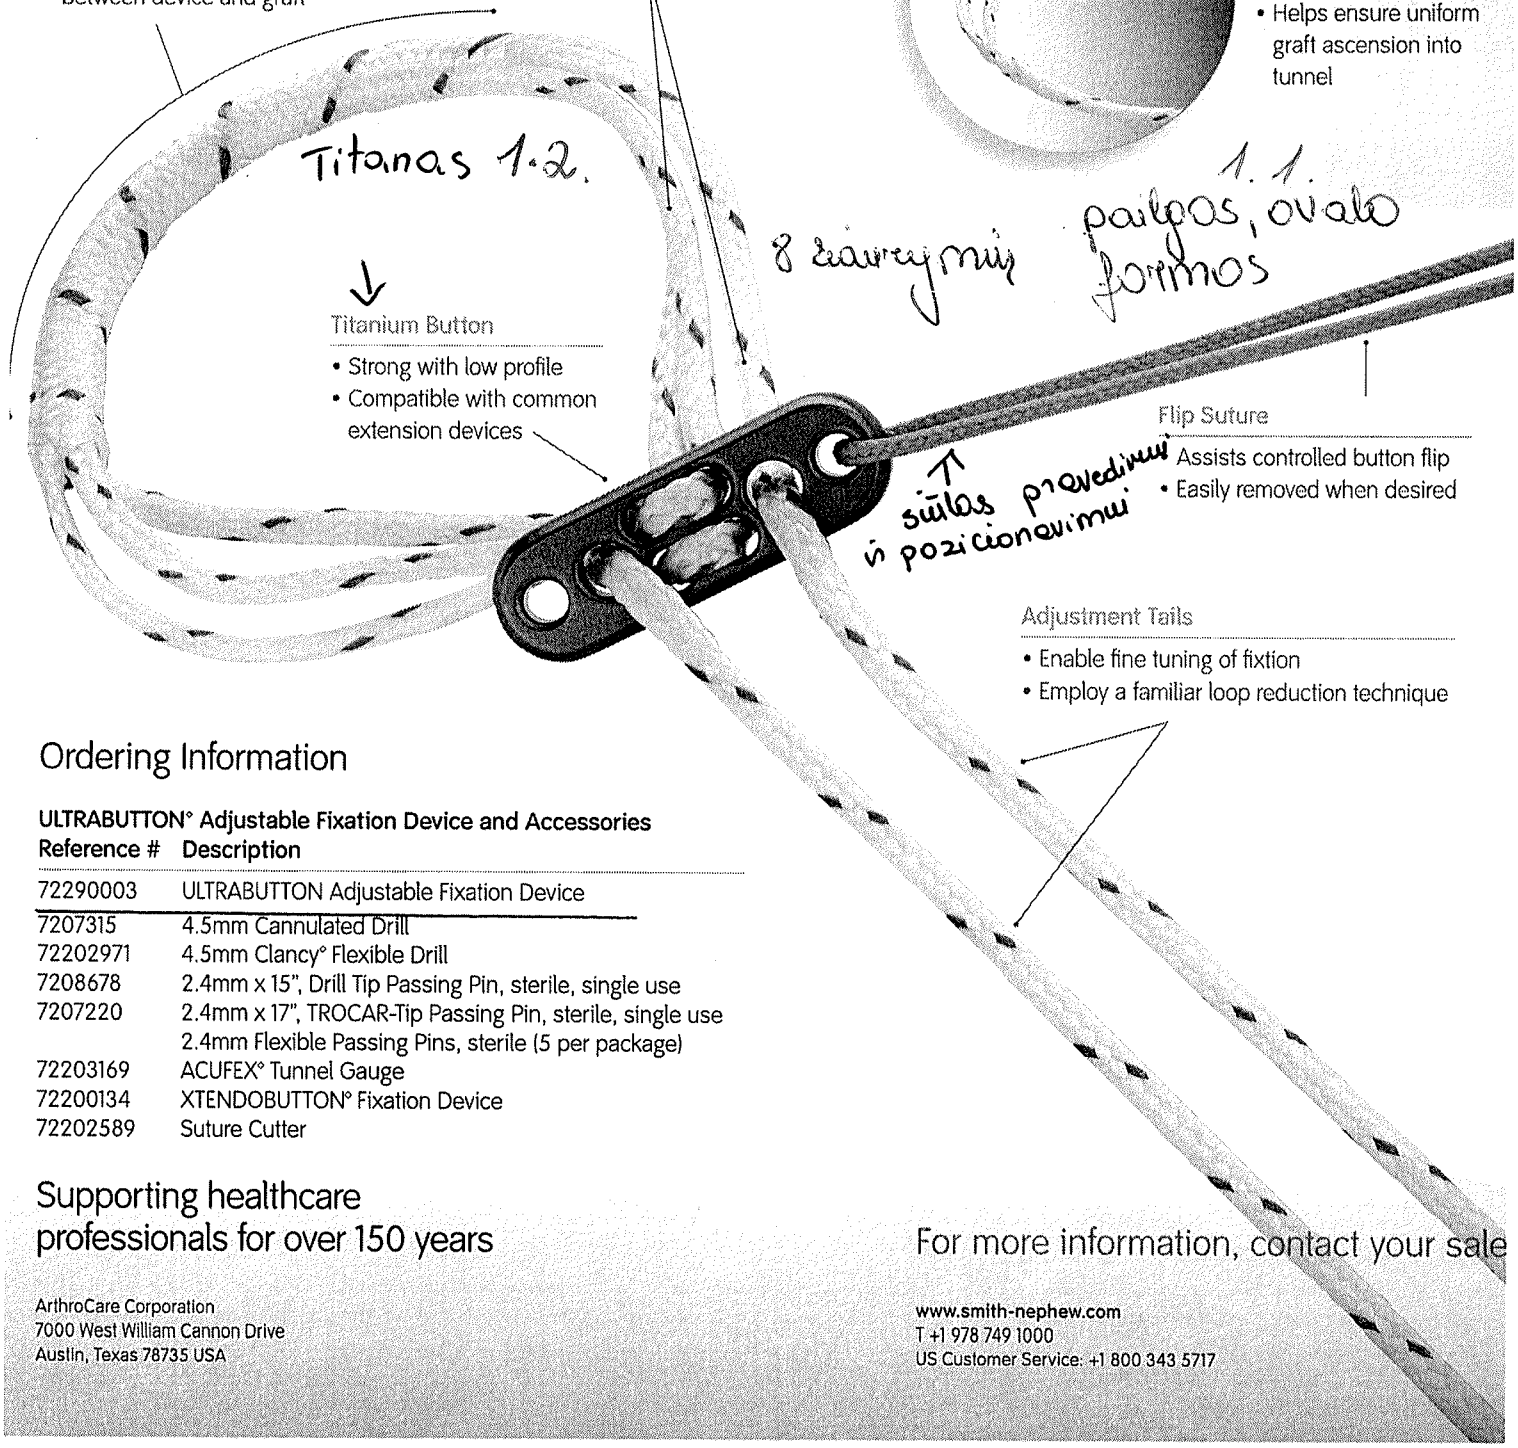

Titanium Button

- Strong with low profile
- Compatible with common extension devices

Flip Suture

- Assists controlled button flip
- Easily removed when desired

Adjustment Tails

- Enable fine tuning of fixtion
- Employ a familiar loop reduction technique

Ordering Information

ULTRABUTTON® Adjustable Fixation Device and Accessories

Reference #	Description
72290003	ULTRABUTTON Adjustable Fixation Device
7207315	4.5mm Cannulated Drill
72202971	4.5mm Clancy® Flexible Drill
7208678	2.4mm x 15", Drill Tip Passing Pin, sterile, single use
7207220	2.4mm x 17", TROCAR-Tip Passing Pin, sterile, single use
	2.4mm Flexible Passing Pins, sterile (5 per package)
72203169	ACUFEX® Tunnel Gauge
72200134	XTENDOBUTTON® Fixation Device
72202589	Suture Cutter

Supporting healthcare professionals for over 150 years

For more information, contact your sale

ArthroCare Corporation
7000 West William Cannon Drive
Austin, Texas 78735 USA

www.smith-nephew.com
T +1 978 749 1000
US Customer Service: +1 800 343 5717

ENDOBUTTION◊ CL ULTRA & ULTRABUTTON◊

smith&nephew

Product Comparison

1.2 Matmenys: ilgis 12 mm, plotis 4 mm.

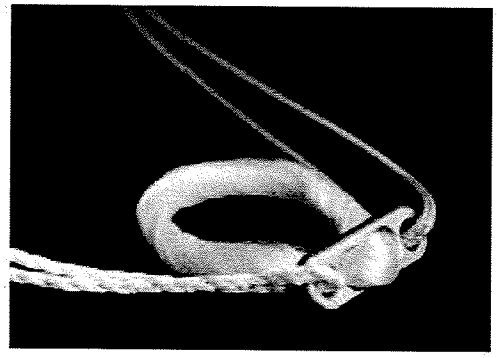

1.2. Savaime užsiveržiantis

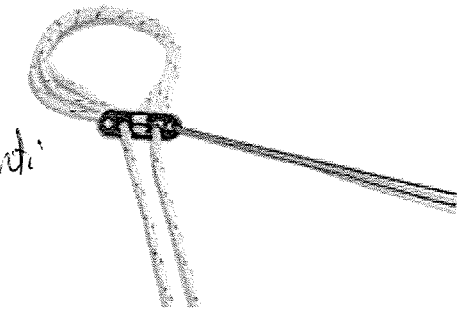

	ENDOBUTTON CL ULTRA Device	ULTRABUTTON Device
Button	L: 12mm; W: 4mm; H: 2mm; 4 holes	Same; 8 holes
	Gold titanium	Blue titanium Titanas 1.2.,
Loop	Polyester	Ultrahigh Molecular Weight Polyethylene (UHMWPE) Aukštos molekulinės masės polietileno pagrindu 1.2.
	Fixed (11 SKUs); 10-60 mm, @ 5 mm	Adjustable (1 SKU); 10 – 105 mm
	Diameter = 5 mm	Diameter = 1.5 mm
Lead	White ULTRABRAID◊ # 5 suture	None – use flip suture
Flip	Green DURABRAID◊ #5 suture	Green #2 polyester suture 1.2 sudaryta iš 2# storio siūlų.
Adjust	None	White/blue adjustment tails

Vertimas iš anglų kalbos

Raičių fiksacinė sistema

1.2. Raištinė ovalo formos, 4 mm x 12 mm išmatavimų, aštuonių kiaurymių titano lydinio "endosaga" skirta medialinės pusės fiksacijai

1.2 Raištinė sistema (kilpa) iš #2 storio siūlų, nesirezorbuojančių iš aukštos molekulinės masės polietileno (UHMWPE). Veikianti savaime užsiveržiančio mazgo principu

1.2 #2 storio siūlas nesirezorbuojantis, iš aukštos molekulinės masės polietileno, skirtas "endosagos" pravedimui.

ULTRABUTTON◊

Adjustable Fixation Device



Graft Protection Sleeve

- Designed to protect graft with large contact area[11]
- Designed to minimize relative motion and sawing effect between device and graft[11]

Interlocking Adjustment

- Maximizes graft in tunnel
- Requires minimal force to reduce loop[23-27]

Flip Suture

- Assists controlled button flip
- Designed for easy removal[11]

1.2 Titanas

Titanium Button

Skintinės spalvos siūlas

1.2 skintas ištraukti sąpi

per kanalą ? ISOT

Adjustment Tails

- Designed to enable fine tuning of fixation

smith&nephew

ULTRABUTTON◊ Device Ordering Information

1.2. savaime užsiverzianti

- ULTRABUTTON◊ Adjustable Fixation Device 72290003
- Non-sterile version of the product **is NOT available**

1.2 néra nesterilios produkto versijos

1

Kopija tikra

LIETUVOS RESPUB

osteca

UAB "Osteca"

11

The ULTRABUTTON Adjustable Fixation Device is versatile and easy to use.

Easy and quick graft loading

Pass the graft through the bottom opening on the backer card and over the graft cradle. Align the graft tails. While holding the circle cutout on the top of the backer card, simply pull down on the graft to disengage from the backer card and the device is now ready for passage.



Convenient button flip visualization

Under direct visualization, use the flip suture to pass the button up the tunnel while applying counter tension on the distal end of the graft with the other hand.

Easy and well-controlled graft passage options

One-handed
Pulling on the tail bridge with a rocking motion helps ensure uniform graft ascension into the tunnel. Maintain counter-tensioning on the distal side of the graft with the other hand.

Two-handed
Pulling on one tail at a time, in small increments each, helps ensure uniform graft ascension into the tunnel and enables the surgeon to use a familiar technique. A second person maintains counter-tension on the distal side

smith&nephew
ULTRABUTTON®
Adjustable Fixation Device

Ultra low displacement, ultra strong fixation and uniquely designed for graft protection.

Endosaga veikianti savaime užsiveržiančio mazgo principu.

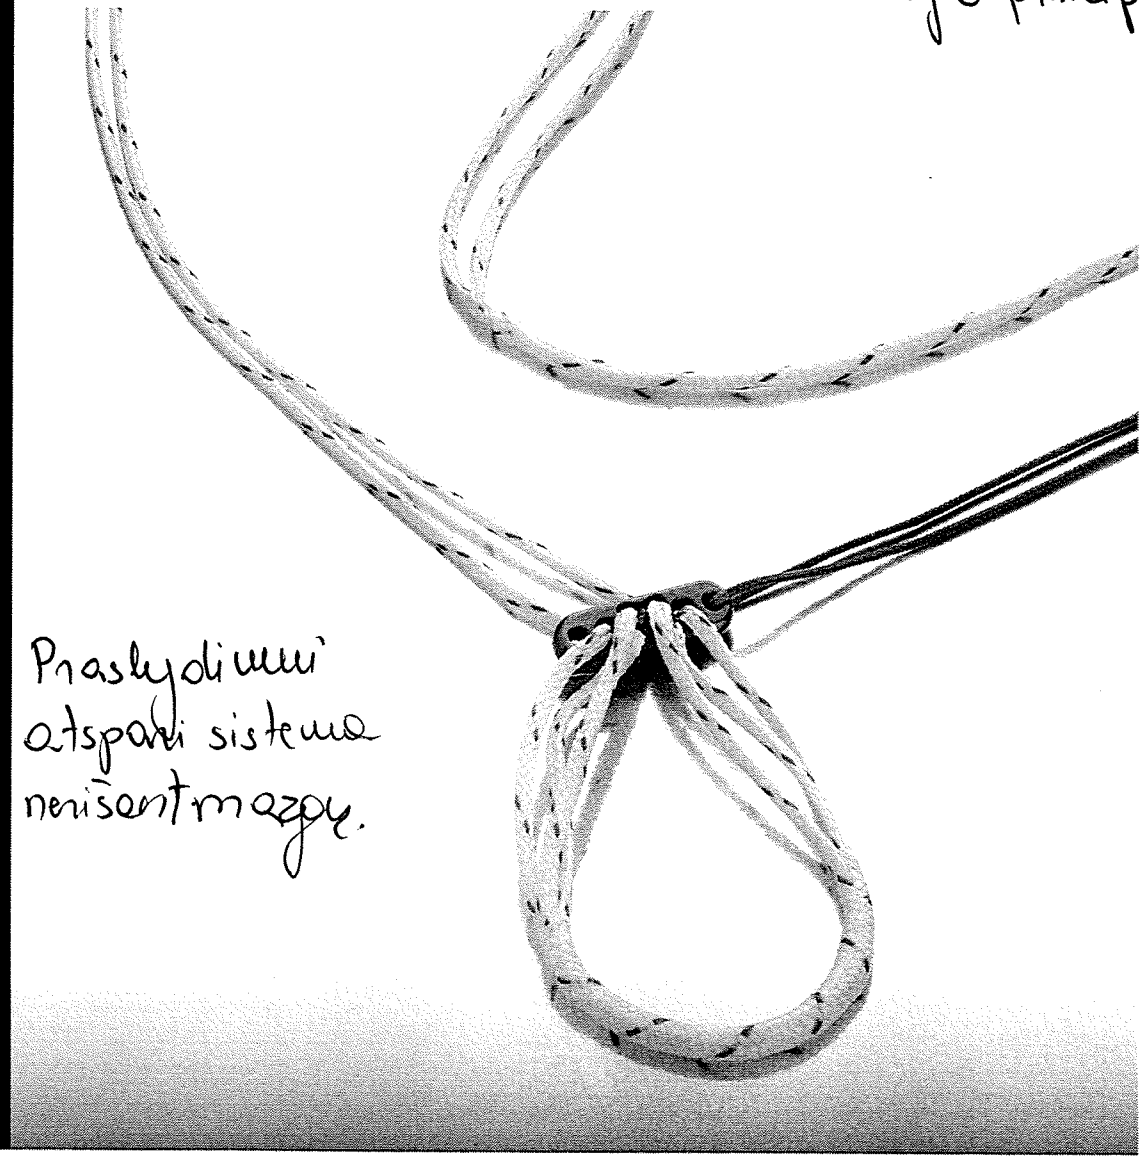

Praslydimui atspari sistema nerišant mazgu.

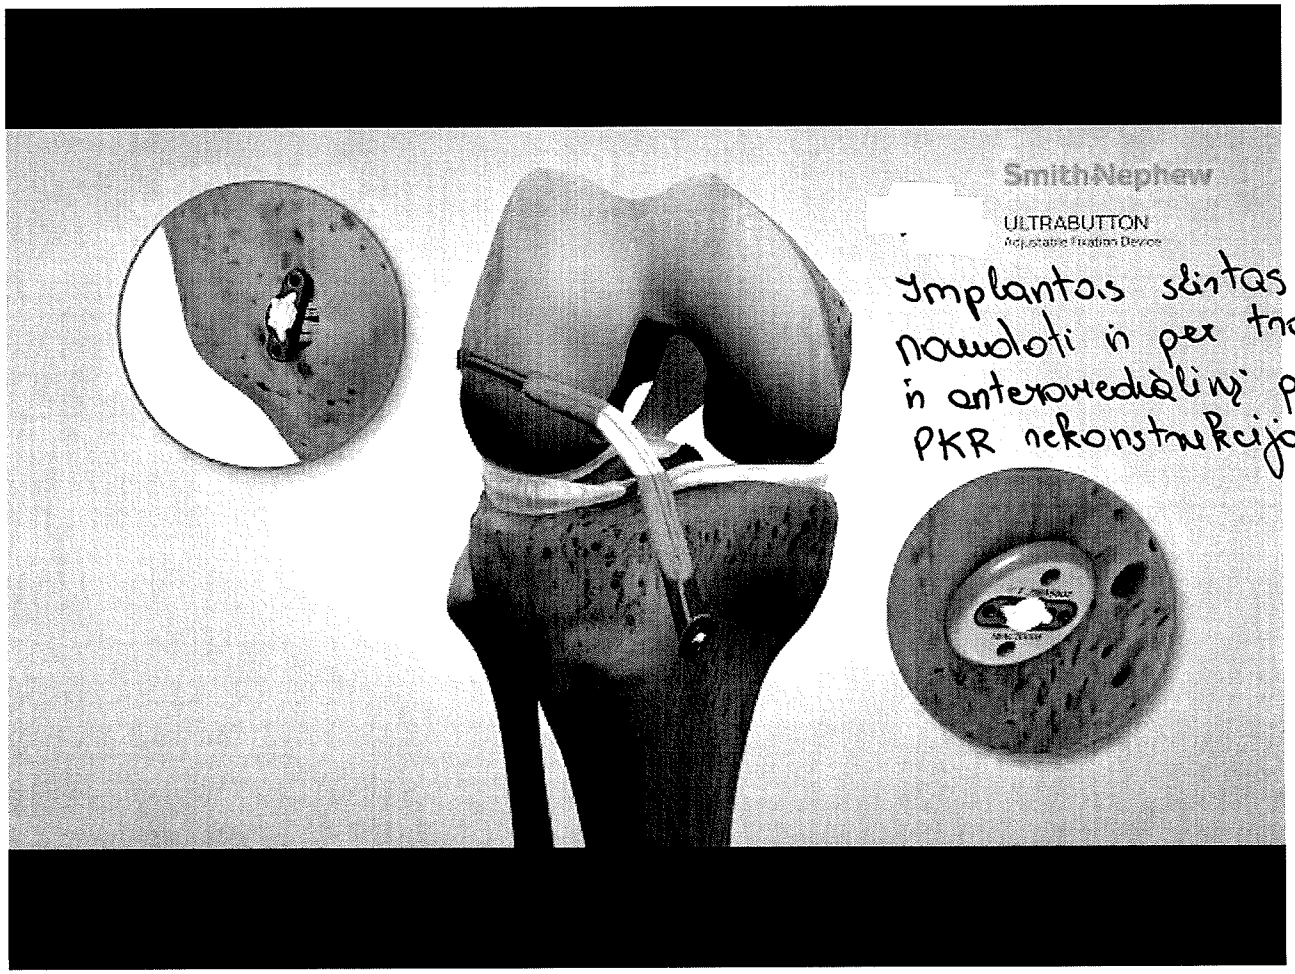

Implantas sintas naudoti in per transtibialinį in anteromedialinį portalus PKR rekonstrukcijos metu.

užtraukiama iš lateralinės žaunikaulio pusės.

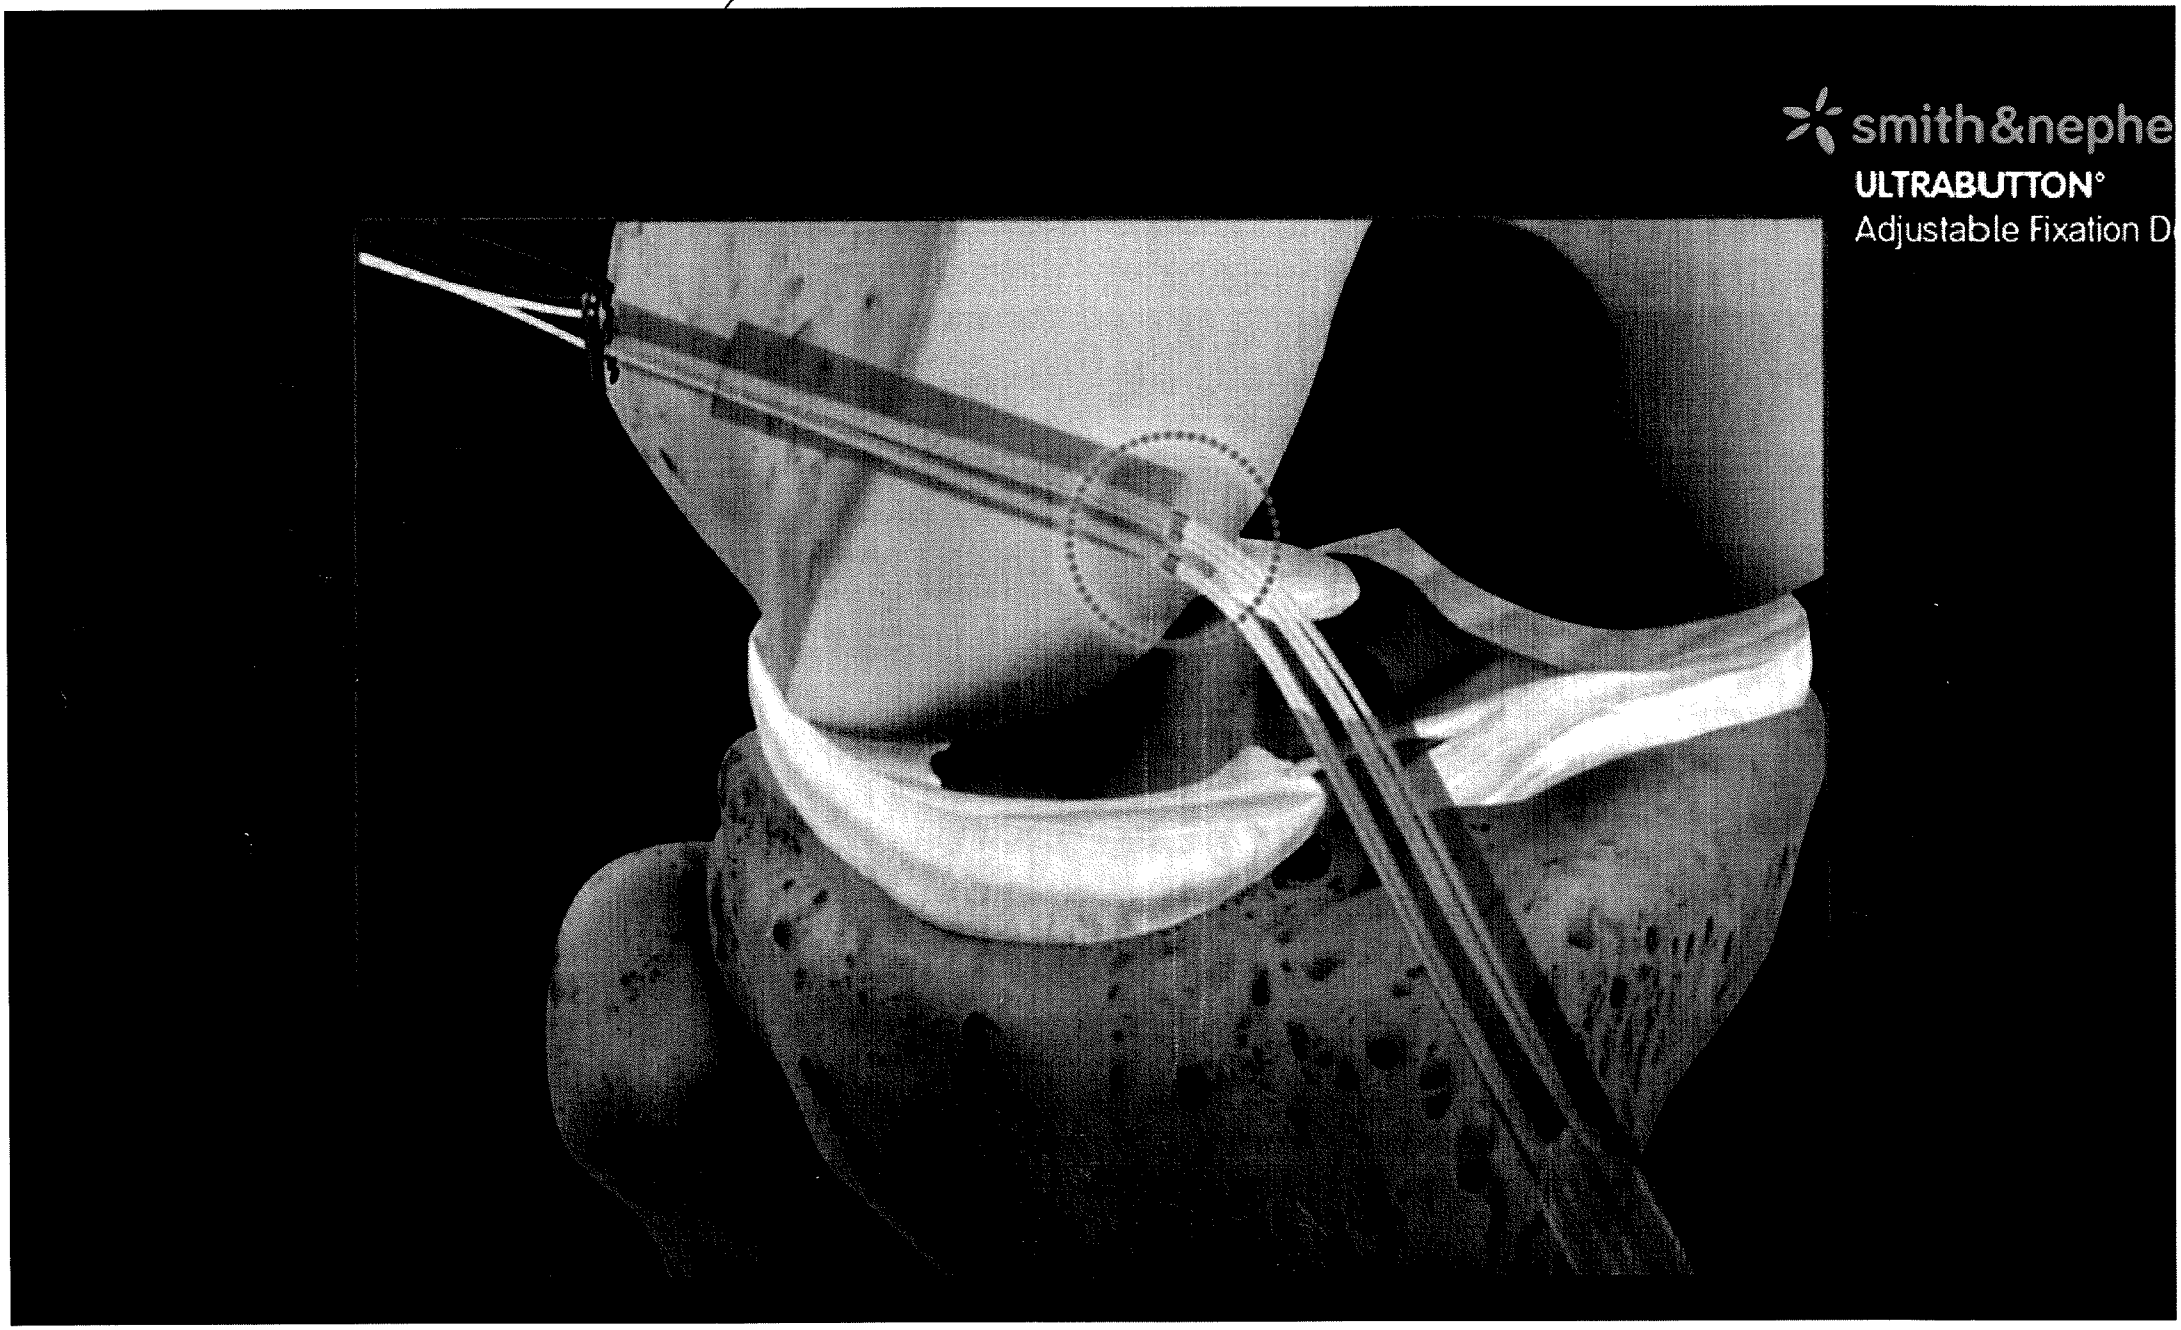

26

12 sterilioje pakuotėje.

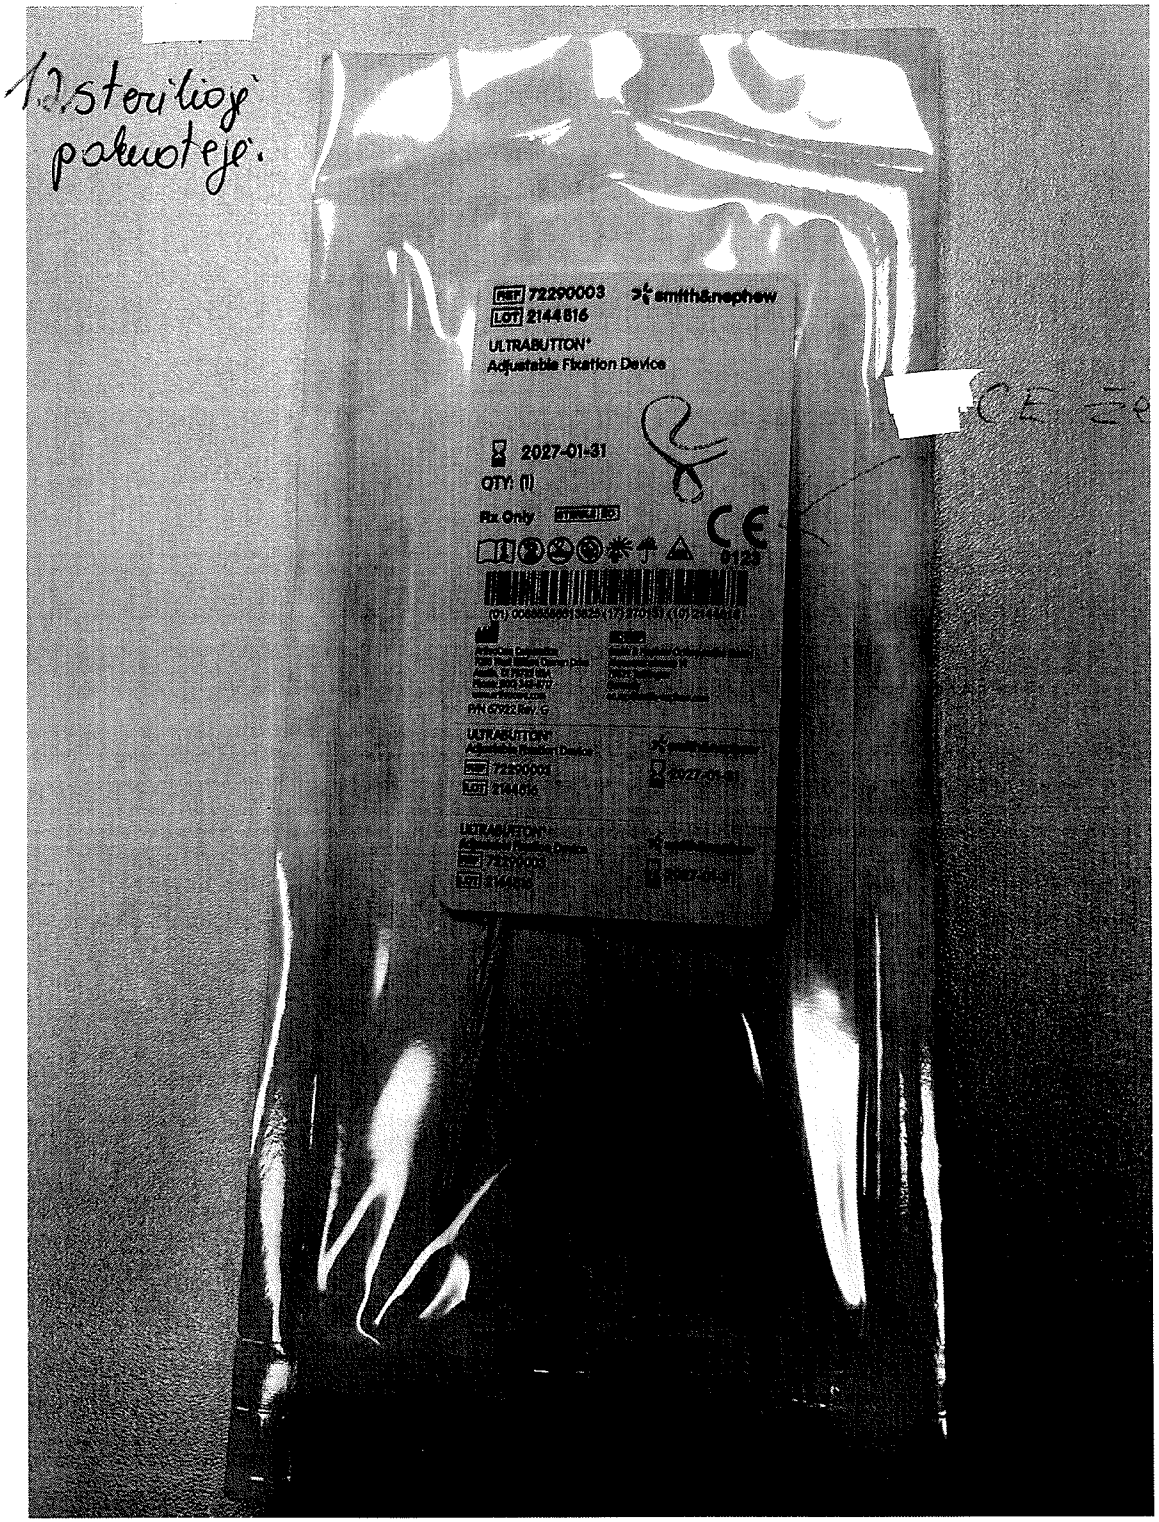

CE ženklas

Single Use Surgical Instruments

② STERILE EO* STERILE R*

Device Description

Smith & Nephew Single Use Surgical Instruments are arthroscopic accessories designed to provide performance for the specific needs of the surgeon. The instruments are provided sterile for single use.

Indications for Use

Smith & Nephew Single Use Surgical Instruments are intended for use in orthopedic surgical procedures.

Contraindications

None known.

⚠ Warnings

Do not use if package is damaged. Do not use if the product sterilization barrier or its packaging is compromised.

- **Contents are sterile unless package is opened or damaged. DO NOT RESTERILIZE. For single use only. Discard any open, unused product. Do not use after the expiration date.**
- **It is the surgeon's responsibility to be familiar with the appropriate surgical techniques prior to use of this device.**
- **Read these instructions completely prior to use.**

Precautions

℞ ONLY U.S. Federal law restricts this device to sale by or on the order of a physician.

- Hazards associated with reuse of this device include, but are not limited to, patient infection and/or device malfunction.
- Prior to use, inspect the device to ensure it is not damaged. Do not use a damaged device.
- Careful attention must be paid to asepsis and avoidance of anatomical hazards.
- As with any surgical instrument, careful attention should be made to assure that excessive force is not placed on the instrument. Excessive forces applied to the instrument can result in failure.
- After use, this device may be a potential biohazard and should be handled in accordance with accepted medical practice and applicable local and national requirements.

Warranty

For single use only. This product is warranted to be free from defects in material and workmanship. Do not reuse.

For Further Information

If further information on this product is needed, contact Smith & Nephew Customer Service at +1 800 343 5717 in the U.S., or an authorized representative.

** Refer to product-specific packaging to determine actual sterilization method.*

©2004, 2020 Smith & Nephew, Inc. All rights reserved.

Nukreipiančiojj viela

REF CATALOG NUMBER 72202998
LOT BATCH CODE 2130007
(1) Nitinol Guidewire, 1.2 mm x 45 cm

smith&nephew

1.3.

Nitinol-Führungsdraht, 1,2mm x 45cm • Fil guide en nitinol, 1,2 x 45cm • Filo guida in Nitinol, 1,2mm x 45cm • Nitinol voerdraad, 1,2mm x 45cm • Alambre guía de nitinol, 1,2mm x 45cm • Ledare av nitinol, 1,2mm x 45cm • Nitinol-ledesonde, 1,2mm x 45cm • Fio-guia de nitinol, 1,2mm x 45cm • Nitinol-guidewire, 1,2mm x 45cm

(01) 00885554017670 (17) 280829 (10) 2130007
(11) 230829

MADE IN USA

Endoscopy
Smith & Nephew, Inc.
150 Minuteman Road
Andover, MA 01810 USA
T + 1 978 749 1000 • F + 1 978 749 1108
Customer Service +1 800 343 5717

USE BY 2028-08-29

STERILE R
IRRADIATION STERILIZED
CE 2797
NO REUSE
Rx only

CONSULT INSTRUCTIONS
CAUTION

* Trademark(s) of Smith & Nephew

E03H63AA, 2

29