

**DICOM CONFORMANCE STATEMENT
FOR
DIAGNOSTIC ULTRASOUND SYSTEM**

Aplio i900

MODEL TUS-AI900 V1.6/V1.7/V1.8

Aplio i800

MODEL TUS-AI800 V1.6/V1.7/V1.8

Aplio i700

MODEL TUS-AI700 V1.6/V1.7/V1.8


CANON MEDICAL SYSTEMS CORPORATION

4. NETWORKING

- 1 pirkimo dalis, p. 21
- 2 pirkimo dalis, p. 8
- 3 pirkimo dalis, p. 6
- 4 pirkimo dalis, p. 16

4.1 IMPLEMENTATION MODEL

4.1.1 Application Data Flow

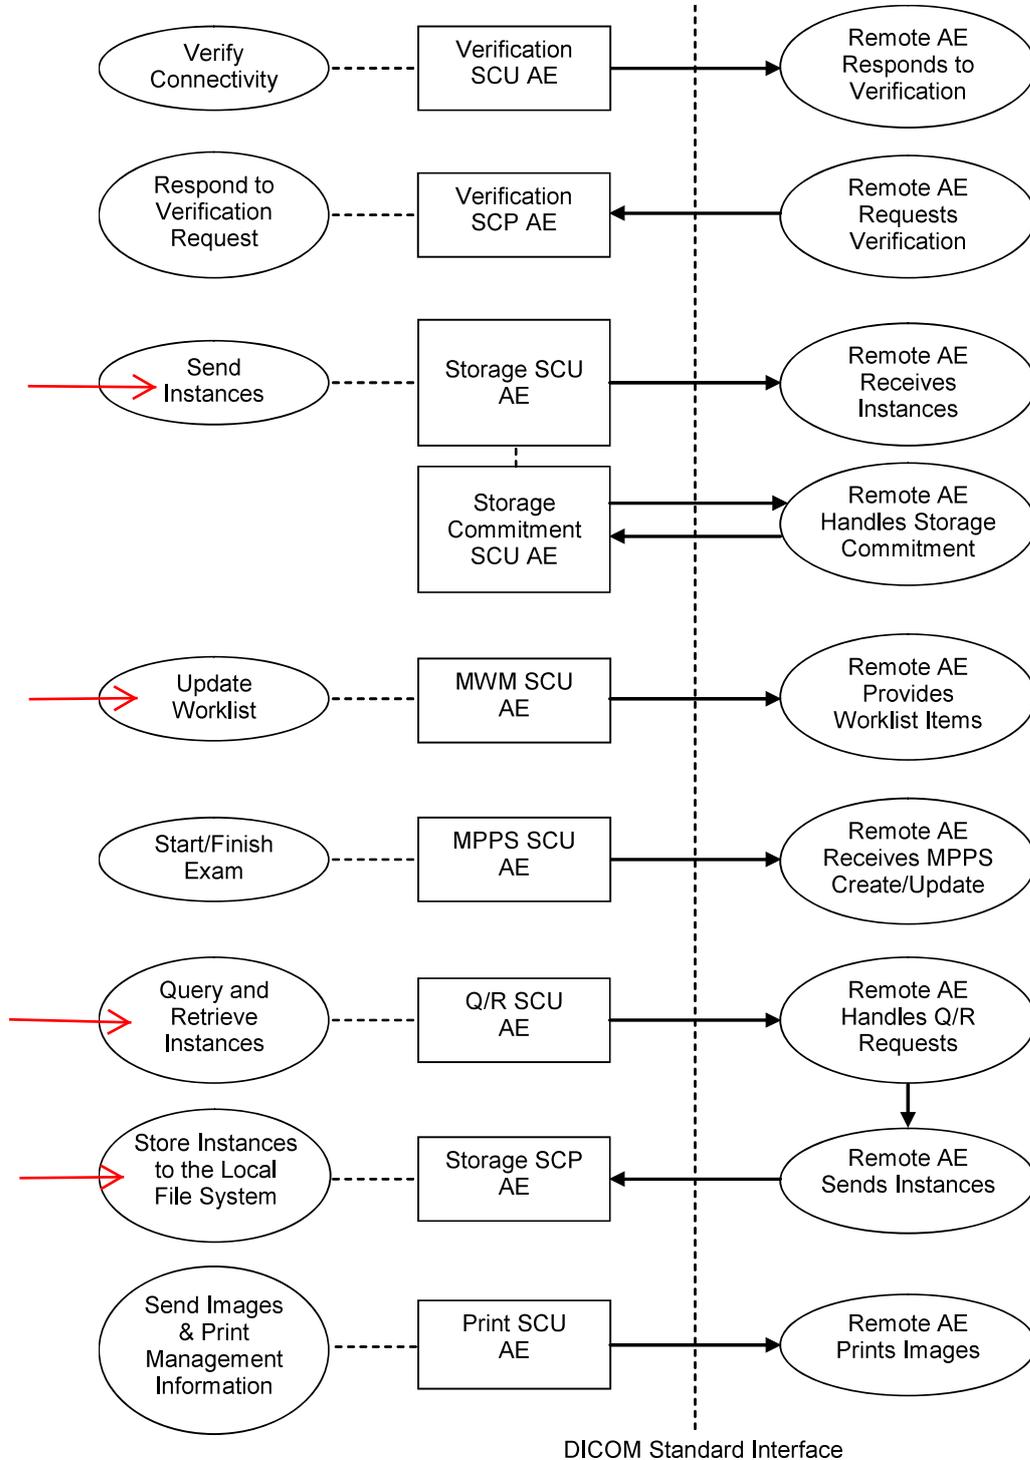

**Figure 4.1-1
APPLICATION DATA FLOW DIAGRAM**