


Balionas, skirtas aortos  
okliuzijai ir aortos protezų  
modeliavimui.

Reliant™  
Stent Graft Balloon Catheter

# EXPAND POSSIBILITIES

The versatile, reliable and conformable solution  
that extends procedural possibilities

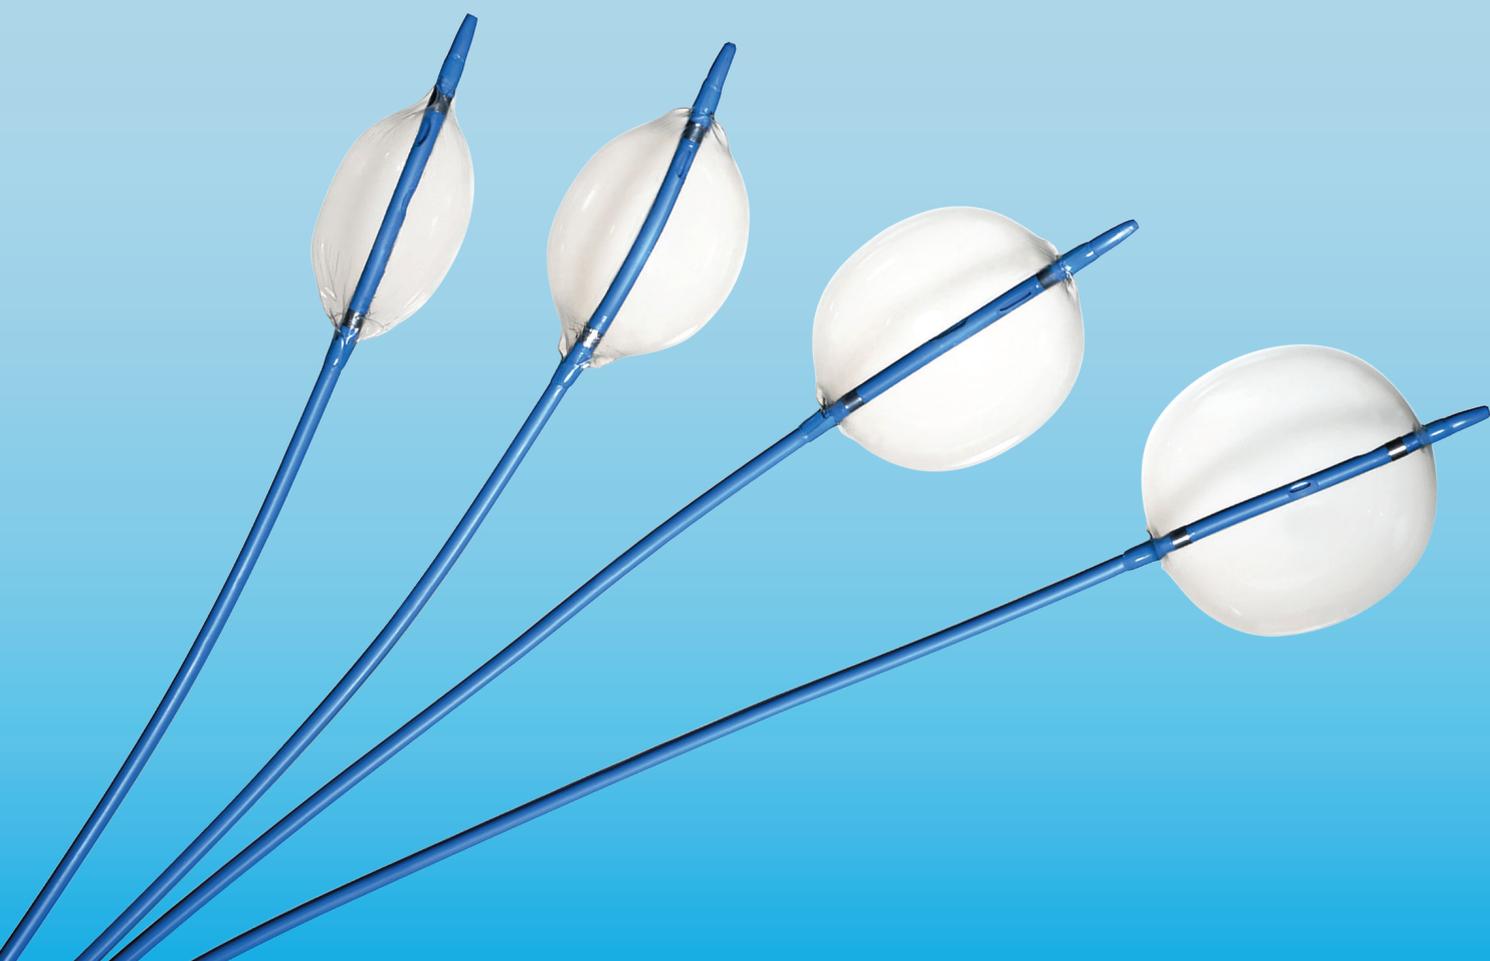

**Medtronic**  
Further, Together

Darbinis baliono kateterio ilgis 100cm.

Usable length: 100 cm

Išplėsto baliono darbinio diametro ribos 10-46mm.

Inflation diameter: 10–46 mm

Introducer sheath: compatible with 12F

Pritaikytas darbui su 12F introduuseriu

Material type: compliant polyurethane (non-latex)<sup>†</sup>


Shaft size: 8F

Guidewire diameter: 0.038"/0.9652 mm or smaller

Pritaikytas darbui su 0,038 ir mažesne<sup>††</sup> viela.


## MULTIPLE TREATMENTS IN A SINGLE BALLOON FOR THORACIC, ABDOMINAL AND ILIAC THERAPIES

Balionas, skirtas aortos okliuzijai ir aortos protezų modeliavimui.



### Versatile Design

- Widest range of inflation diameters in a single low profile balloon able to treat thoracic to iliacs (10 mm–46 mm)<sup>‡</sup>
- Compatible with 12F sheath



### Reliable Performance

- Consistent inflation and deflation time
- Stable expansion with minimum balloon overhang to reduce risk of vessel trauma
- Dependable expansion even after multiple inflations and deflations<sup>§</sup>



### Improved Conformability

- Expands kinks and smooths creases from the graft material
- Compliant balloon expansion

Balionas visiškai adaptatyvus (angl. Full compliant)

### Clinical Uses Include:

- For use in thoracic, abdominal and iliac endograft procedures
- Endograft molding
- Apposition of endografts in seal zones
- Temporary aortic occlusion

BALLOON INFLATION TABLE		
46 mm Balloon		
Diameter (mm)	mL (cc)	
10	3	
20	9	
30	19	
40	41	
46 <sup>†</sup>	60	

CAUTION: This table is only a guide. Balloon expansion should be carefully monitored under fluoroscopy. Do not exceed maximum inflation diameter (46 mm). Rupture of balloon may occur.

### PRODUCT ORDERING INFORMATION

Product Code	Inflation Diameter (mm)	Shaft Size (F)	Usable Length (cm)	Sheath Compatibility (F)
AB46	10–46	8	100	12

<sup>†</sup> Does not contain latex.

<sup>‡</sup> Reliant™ Stent Graft Balloon Catheter Instructions for Use, Cook Coda™ Balloon Catheter Instructions for Use, Gore Tri-Lobe™ Instructions for Use.

<sup>§</sup> Data on file Medtronic. Maximum of 20 inflations, deflations.

<sup>†</sup> Maximum inflation diameter.

**Important Information:** [www.medtronic.com/manuals](http://www.medtronic.com/manuals).

Consult instructions for use at this website. Manuals can be viewed using a current version of any major internet browser. For best results, use Adobe Acrobat® Reader with the browser.

# Medtronic

**Invatec S.p.A.**  
Via Martiri della Libertà 7  
25030 Roncadelle (BS)  
Italy  
Tel: +39.030.2589311

**Medtronic**  
710 Medtronic Parkway NE  
Minneapolis, MN 55432  
USA  
Tel: +1.763.514.4000

**Medtronic International Trading Sàrl**  
Route du Molliou 31  
CH-1131 Tolochenaz  
Switzerland  
Tel: +41.21.802.7000

**Medtronic of Canada Ltd.**  
99 Hereford Street  
Brampton, Ontario L6Y 0R3  
Canada  
Tel: +1.905.460.3800

**Medtronic Latin America**  
3750 NW 87th Avenue, Suite 700  
Miami, FL 33178  
USA  
Tel: +1.786.709.4200

**Medtronic International Ltd.**  
49 Changi South Avenue 2  
Singapore 486056  
Tel: +65.6436.5000

**Medtronic Australasia Pty Ltd.**  
97 Waterloo Road  
North Ryde, NSW 2113  
Australia  
Tel: +61.29857.9000

**Medtronic New Zealand**  
Unit N16, Mezzanine Level 5  
Gloucester Park Road  
Onehunga  
Auckland  
New Zealand

**Medtronic Korea Co., Ltd.**  
5F, Sajo Building  
1001 Daechi-dong, Kangnam-ku  
Seoul, 135-280  
Korea  
Tel: +82.2.3404.3600

**Medtronic META FZ-LLC**  
Office Park, Block D, 2nd Floor  
PO Box 500638  
Dubai Internet City | Dubai,  
United Arab Emirates  
Tel: +971.4.818.2666

[medtronic.com/aortic](http://medtronic.com/aortic)