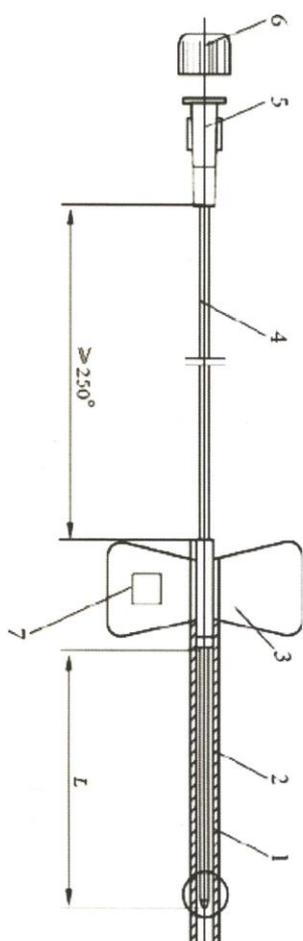
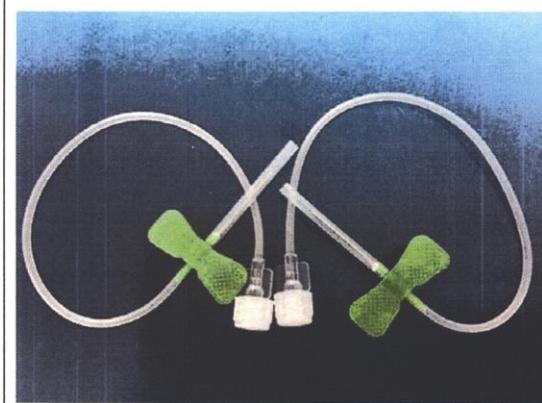


## TECHNICAL SPECIFICATION OF SCALP VEIN SET

<ul style="list-style-type: none"> <li>- Materials: medical PVC + ABS + PE + stainless steel</li> <li>- Size: 18G, 19G, 20G, 21G, 22G, 23G, 24G, 25G, 26G, 27G, 28G x 1" or 3/4"</li> <li>- Tubing length: 30cm</li> </ul>	<ul style="list-style-type: none"> <li>- Non-pyrogenic</li> <li>- Latex free</li> <li>- For single use</li> <li>- ETO sterilized</li> </ul> <div style="text-align: right; font-size: 2em; font-weight: bold;">CE</div> <div style="text-align: right; font-size: 1em;">0197</div>																								
	<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 10%;">No.</th> <th style="width: 60%;">Designation</th> <th style="width: 30%;">Materials</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>Protective sheath</td> <td>PE</td> </tr> <tr> <td>2</td> <td>Needle cannula</td> <td>Stainless steel</td> </tr> <tr> <td>3</td> <td>Wings</td> <td>ABS</td> </tr> <tr> <td>4</td> <td>Tubing</td> <td>PVC</td> </tr> <tr> <td>5</td> <td>Luer lock</td> <td>ABS</td> </tr> <tr> <td>6</td> <td>Luer lock cap</td> <td>PE</td> </tr> <tr> <td>7</td> <td>Needle size</td> <td></td> </tr> </tbody> </table> <div style="text-align: center; margin-top: 10px;">  </div>	No.	Designation	Materials	1	Protective sheath	PE	2	Needle cannula	Stainless steel	3	Wings	ABS	4	Tubing	PVC	5	Luer lock	ABS	6	Luer lock cap	PE	7	Needle size	
No.	Designation	Materials																							
1	Protective sheath	PE																							
2	Needle cannula	Stainless steel																							
3	Wings	ABS																							
4	Tubing	PVC																							
5	Luer lock	ABS																							
6	Luer lock cap	PE																							
7	Needle size																								

### PACKING:

1. Individual PE bag
2. Packing is adapted to the ethylene oxide sterilization. The cover mentions the necessary indications for content identification: designation, item code, manufacture date and expire date and lot number.
3. Packing details: 1pc/PE bag, 100pcs/box

### QUALITY:

1. The product quality is guaranteed by inspections at all levels of manufacture, all our products are manufactured in 100,000 grade clean room, the final control is made at the level of packaging.
2. The packaged scalp vein set is sterilized by ethylene oxide according to a validated method in the physical and microbiological field. The shelf life is 5 years from the manufacture date.
3. The product conforms to MDD 93/42/EEC amended by 2007/47/EC and maintains a quality assurance system according to ISO 13485.

Vertimas iš anglų kalbos

VIENKARTINĖS ADATOS „BUTTERFLY“ TECHNINĖ SPECIFIKACIJA -  
APRAŠYMAS

Žaliavos PVC + ABS + PE + nerūdijantis plienas Dydžiai: 18G, 19G, 20G, 21G, 22G, 23G, 24G, 25G, 26G, 27G, 28G x 1''(2,54cm) arba 3/4'' / (1,9) cm - vamzdelio ilgis - 30cm	- Nepirogeniškos - Be latekso - Vienkartinio naudojimo - Sterilizuota EO  garais 0197		
Žr. techn, dok. brėžinius	Nr.	Žymuo	Medžiaga
	1	Apsauginis futliaras	PE
	2	Adatos kaniulė	Nerūdijantis plienas
	3	Sparneliai	ABS
	4	Vamzdelis	PVC
	5	Luer lock jungtis	ABS
	6	Luer lock jungties dangtelis	PE
	7	Adatos dydis	26G, 27G, 28G x 1'' ( 2,54cm arba 1,9 cm )

PAKUOTĖ:

1. Individuali PE pakuotė
2. Pakuotė pritaikyta sterilizuoti etileno oksidu. Viršelyje minimos būtinos turinio identifikavimo nuorodos: pavadinimas, prekės kodas, pagaminimo data ir galiojimo pabaigos data bei partijos numeris.
3. Pakuotės informacija: 1 vnt / PE pakuotė, 100 vnt / dėžutė

KOKYBĖ:

1. Produktų kokybę garantuoja patikrinimai visais gamybos lygiais, visi mūsų produktai yra gaminami 100 000 klasės švarioje patalpoje, o galutinė kontrolė atliekama pakuočių lygyje.
2. Supakuotos adatos sterilizuojamas etileno oksidu pagal patvirtintą metodą fiziniame ir mikrobiologiniame srityje. Galiojimo laikas yra 5 metai nuo pagaminimo dienos.
3. Produktas atitinka MDD 93/42 / EEB su pakeitimais, padarytais 2007/47 / EB, ir palaiko kokybės užtikrinimo sistemą pagal ISO 13485

Už vertimą atsakingas A. Zapalskio IĮ „AZAS“ direktorius



Juozas Devižis