


# Knitted Vascular Prosthesis

Impregnuotos megztos dirbtinés kraujagyslés

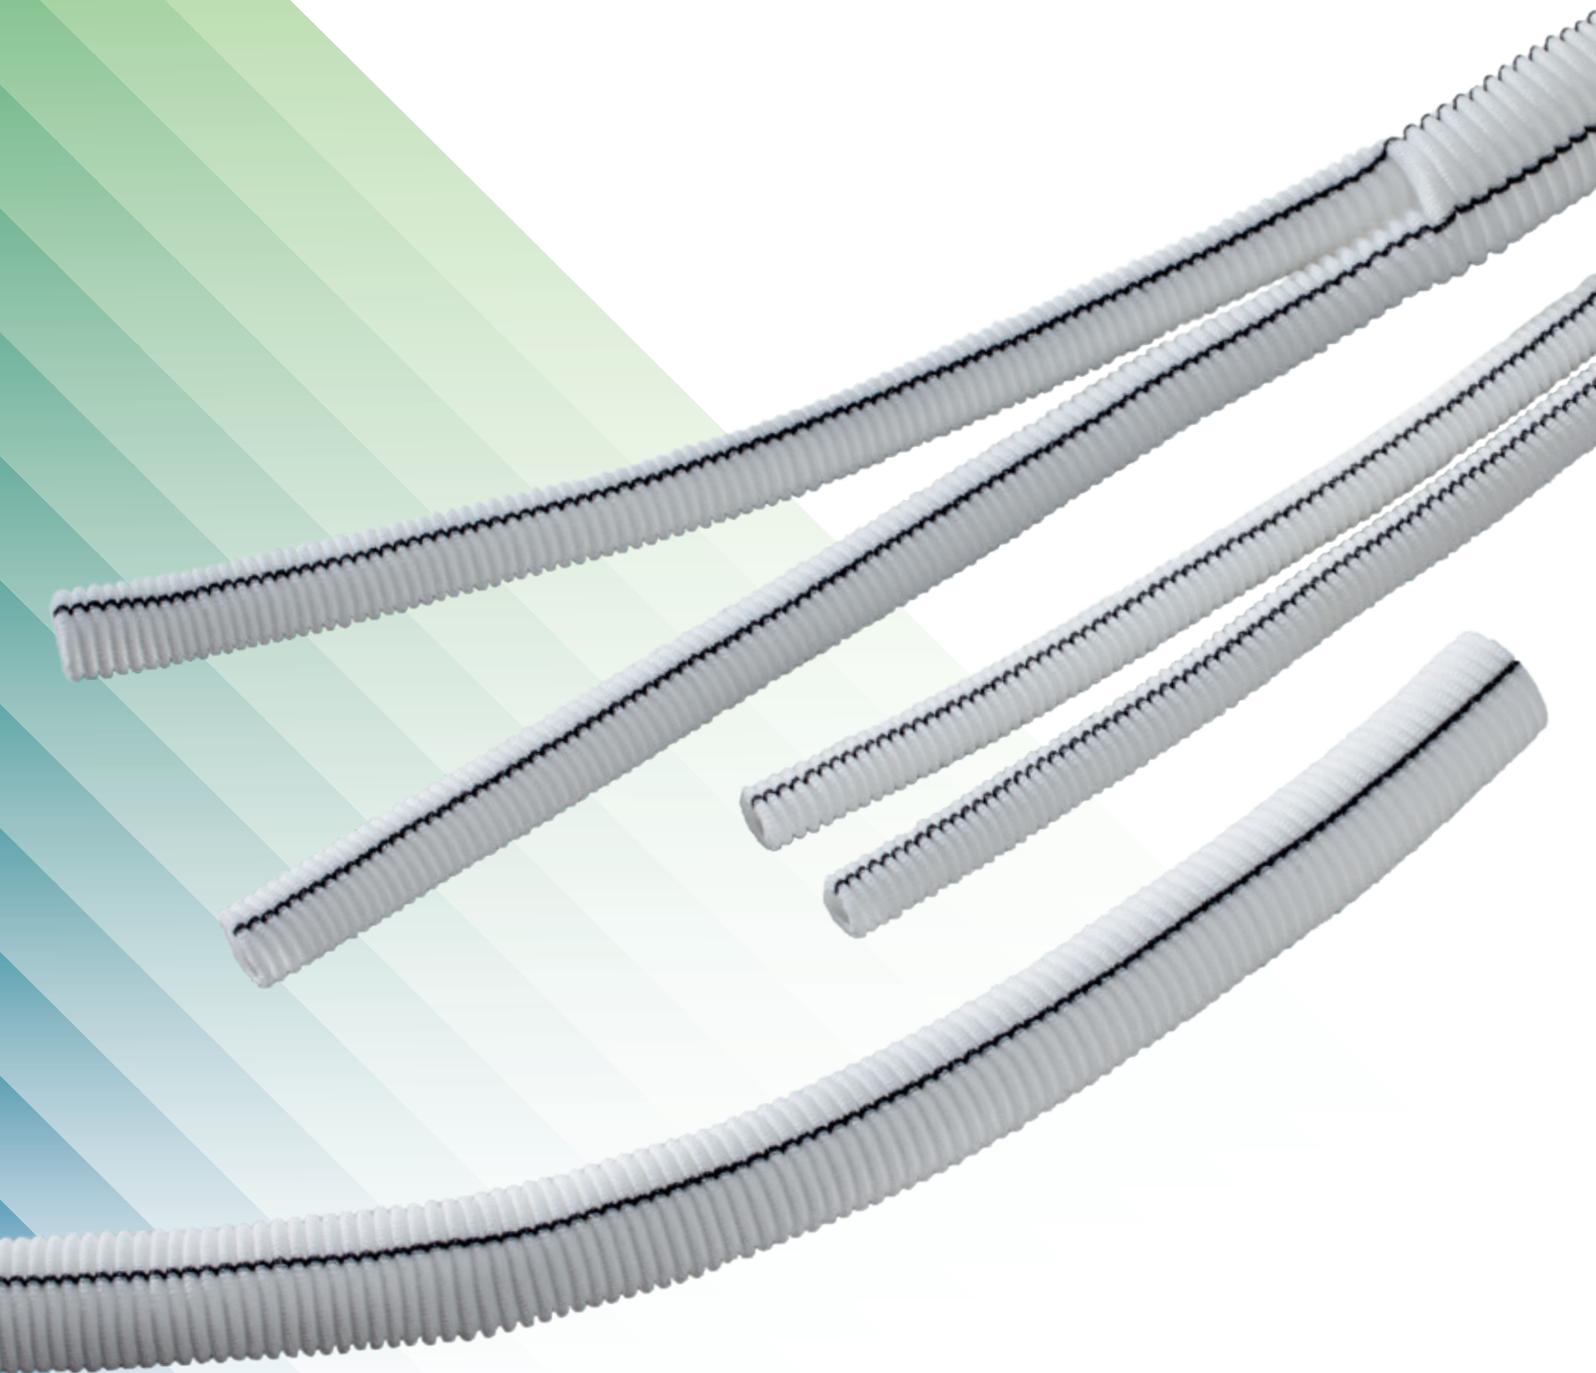

# FlowNit Bioseal

## Knitted vascular prostheses:

- Specific knitting techniques for high burst resistance and low dilatation<sup>12</sup> **impregnuotos kolagenu**
- Aldehyde and isocyanate free BIOSEAL impregnation using dehydrothermal crosslinked collagen guarantees primary sealing of the blood in the prosthesis<sup>3</sup>
- Concentric crimping and the guide line allow precise positioning of the prosthesis
- Soft and supple texture for easy handling

## Ordering Information

### Straight prostheses

Catalogue No.	Ø (mm)	Length (cm)
35ST1506	6	15
35ST3006	6	30
35ST6006	6	60
35ST1507	7	15
35ST3007	7	30
35ST6007	7	60
35ST1508	8	15
35ST3008	8	30
35ST6008	8	60
35ST0008	8	100
35ST1510	10	15
35ST3010	10	30
35ST6010	10	60
35ST0010	10	100

### Straight prostheses


Catalogue No.	Ø (mm)	Length (cm)
35ST1512	12	15
35ST3012	12	30
35ST1514	14	15
35ST3014	14	30
35ST1516	16	15
35ST3016	16	30
35ST1518	18	15
35ST3018	18	30
35ST1520	20	15
35ST3020	20	30
35ST1522	22	15
35ST3022	22	30
35ST1524	24	15
35ST3024	24	30

### Bifurcated prostheses

Catalogue No.	Ø (mm)	Length (cm)
35BI1206	12x6	45
35BI1407	14x7	45
35BI1608	16x8	45
35BI1809	18x9	45
35BI2010	20x10	45
35BI2211	22x11	45
35BI2412	24x12	45

7d.

6d.



# ARTIVION™

Learn more at [artivion.com](http://artivion.com)

#### References:

- 1 JOTEC GmbH, subsidiary of CryoLife, Inc.: Internal mechanical test data
- 2 Bell C-M.: [Study on the issue of expansion of textile implants] - (internal data, JOTEC GmbH)
- 3 Freischlag J, J.A. and Moore, W. S.: Clinical Experience with a Collagen-Impregnated Knitted Dacron Vascular Graft; Ann of Vascular Surg 1990; 4(5): 449-454

Indications: FlowNit Bioseal is indicated in arterial aneurysms and vascular occlusions. FlowNit BIOSEAL is primarily indicated for vascular replacement in the entire abdominal aorta and in peripheral vascular applications involving vessel diameters of at least 6 mm.

All products and indications are not available/approved in all markets. All trademarks are owned by Artivion, Inc. or its subsidiaries. On-X Life Technologies, Inc. Jotec GmbH and Ascyrus Medical GmbH are wholly owned subsidiaries of Artivion, Inc. © 2022 Artivion, Inc. All rights reserved.

**Artivion, Inc.**  
 1655 Roberts Blvd., NW  
 Kennesaw, GA 30144 USA  
 Phone: +1-888-427-9654  
 Fax: +770-590-3753  
 E-mail: [inquiries@artivion.com](mailto:inquiries@artivion.com)  
 For contact information by region, please visit. [www.artivion.com/contact](http://www.artivion.com/contact)

 JOTEC GmbH, Lotzenäcker 23, 72379 Hechingen, Germany

JT-BR-0350200-EN V03 11/2022